


Operation Manual

Microtector III G888

1 to 7 gas warning devices

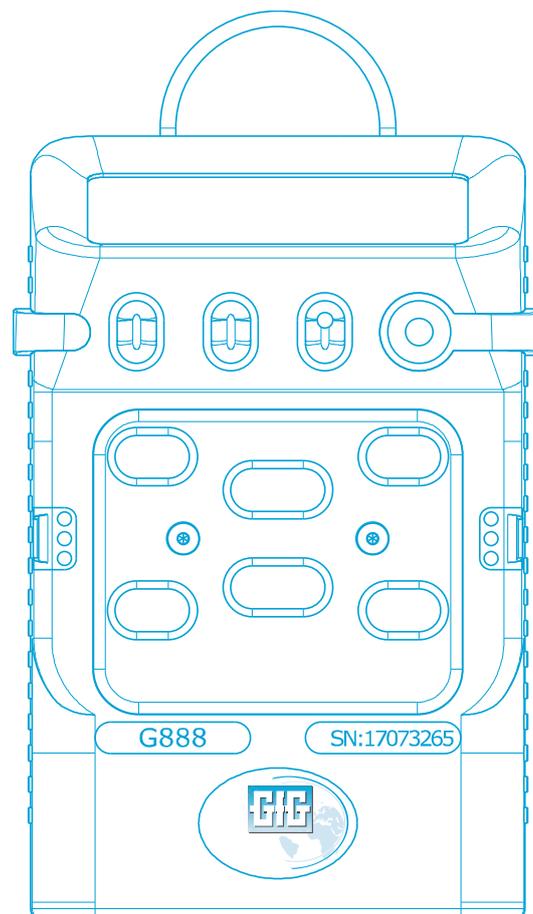

Measurable safety by using GfG devices

Congratulations!

You have chosen a precision instrument made by GfG.
A very good choice!

Since reliability, safety, optimum performance and efficiency distinguish our devices.

They comply with the national and international directives.

These operating instructions will help you to rapidly and safely operate the device.

Please strictly follow our operating instructions before commissioning!

Our employees will be at your service at any time in case of inquiries.

Yours

GfG Gesellschaft für Gerätebau mbH

Klönnestraße 99

D-44143 Dortmund

Phone: +49(0)231 - 564 00-0

Fax: +49(0)231 - 51 63 13

E-mail: info@gfg-mbh.com

Internet: www.gasmessung.de

Table of contents

	Page
1 INTRODUCTION	5
1.1 For your safety	5
1.2 Area of use and application	5
1.3 Special conditions for the safe use	5
1.4 Design	6
2 OPERATING INSTRUCTIONS	7
2.1 Commissioning	7
2.1.1 Switching the device on and off	7
2.1.2 Other messages when starting the device	8
2.2 Measuring mode	8
2.2.1 Display of the measured values, icons and key functions	8
2.2.2 Monitoring and gas alarms	9
2.2.3 Acknowledging the gas alarms	9
2.2.4 Battery capacity and battery alarm	10
2.2.5 Motion detection and Man-Down Alarm	10
2.2.6 Short-term, Long term, Maximum, Minimum values	10
2.2.7 Zoom display and detail view	10
2.2.8 Peak display of the peak values	11
2.2.9 Turning the display	11
2.2.10 Use of the flashlight	11
2.2.11 Display lighting	11
2.2.12 Peculiarities when monitoring in the LEL range	11
2.2.13 Influence of oxygen and interference gases	12
2.2.14 Recording of measurement data with the data logger	12
2.2.15 Wireless data transfer	12
2.3 Service mode	12
2.3.1 Main menu	13
2.3.1.1 Place – Choice of a measuring point	13
2.3.1.2 Name – Choice of a device user	13
2.3.1.3 AutoCal – Menu for AutoCal adjustment	13
2.3.1.4 Sensor overview	14
2.3.1.5 System information	14
2.3.2 Service menu	14
2.3.2.1 System menu for system settings	15
2.3.2.1.1 Bump test	15
2.3.2.1.2 Sensor adjustment (zero point and calibration)	15
2.3.2.1.3 Maintenance	15
2.3.2.1.4 Time	16
2.3.2.1.5 System options	16
2.3.2.1.6 Sensor choice – activation / deactivation of sensors	17
2.3.2.1.7 AutoCal air - Sensor release for AutoCal adjustment	17
2.3.2.1.8 AutoCal gas sensor release for AutoCal adjustment	17
2.3.2.2 Sensor menu for sensor settings	17
2.3.2.2.1 Zero - Adjusting the zero point	18
2.3.2.2.2 Calibrating - Sensitivity adjustment	18
2.3.2.2.3 Alarms - Alarm setting	19
2.3.2.2.4 Calibration data	19
2.3.2.2.5 Information	19
2.3.2.2.6 Measuring range	20
2.3.2.3 Data logger settings	20
2.4 Energy supply	21
2.4.1 Charging the device battery	21
2.4.2 Removal of the lazy battery effect on a device battery	22
2.4.3 Replacing the device battery (NiMH supply unit)	22
3 ANNEX	23
3.1 Maintenance	23
3.2 Maintenance and inspection	23
3.3 Maintenance - Repair	23
3.4 Calibration device	23
3.5 Inspection with the docking station DS400	24
3.6 Malfunction, cause, remedy	24
3.7 Accessories and spare parts	25
3.8 Indications regarding the environmentally friendly disposal	26

3.9	Sensor types and measuring ranges	26
3.10	Sensor specification	27
3.11	Alarm limit values - Basic setting	32
3.12	Technical data	33
3.13	EC Declaration of conformity and EC Type examination certificate	34

1 Introduction

1.1 For your safety

These operating instructions point to the intended use of the product and serve to avoid dangers according to § 3 of the Product Safety Act. It must be read and observed by everyone who operates, services, maintains and inspects this product. This particularly applies for the safety notes in these operating manual which are marked with the icon . This device can serve its intended purpose only if it is operated, serviced, maintained and inspected according to the instructions given by the Gesellschaft für Gerätebau mbH. The warranty assumed by the company GfG Gesellschaft für Gerätebau mbH forfeits, if it is not used, cared for, maintained and controlled according to the specifications of the company GfG.

The above mentioned does not change the indications about the warranty and liability in the sales and delivery conditions of the company GfG. Any repair works may only be performed by professionals or assigned employees. Any conversions and modifications on the product may only be performed with the approval of the GfG. Any unauthorised changes on the product exclude a liability for damages. Only use accessories made by the GfG together with the product. Use the spare parts released by the GfG for any repairs.

A functional test **has to** be performed on every working day before each use - a calibration and, if applicable, an adjustment needs to be performed every 4 months.

1.2 Area of use and application

The G888 is a hand-held meter which serves for the personal protection against dangers caused by toxic or explosive gases and vapours as well as by lack of or excess oxygen. The G888 permanently measures in the diffusion mode and warns the employee carrying the device in case of an occurring gas hazard with a visual and acoustical alarm.

The G888 has been tested by the DEKRA EXAM GmbH concerning the use in potentially explosive atmospheres and possesses a corresponding EU type examination certificate according to the directive 2014/34/EU as well as an IECEx certificate.

Certificates: **BVS 15 ATEX E 064 X**
IECEX BVS 15.0056 X

Labelling: **G888C**  I M2 Ex ia db I Mb  II 2G Ex ia db IIC T4 Gb -20°C≤Ta≤+50°C

1.3 Special conditions for the safe use




Caution: If the device is used in potentially explosive areas or the group I (mining), the G888 needs to be used as intended. I.e. the device needs to be carried on the body and must not be deposited unattended in order to avoid mechanic stress by impacts. It is intended for the low degree of mechanic danger according to the EN 60079-0. The gas measurement device has to be immediately removed for the potentially explosive area and has to be cleaned, if it is soiled with oils and greases or hydraulic fluid.

Before each use, it is necessary to check the gas readings of flammable gases and vapours for zero gas and for test gas. If the gas readings show a continuous zero offset in an environment exempted from measuring gas (fresh air), a zero point adjustment needs to be performed.

In particular after a heavy impact, the zero points of the sensors need to be controlled and readjusted, if required. If the catalytic combustion sensor would cause that the measuring range has been exceeded "" due to an impact stress, this alarm needs to be acknowledged with fresh air and, if applicable, the zero point needs to be readjusted.

If the G888 is being operated without interruption for more than one day, it should be switched off and on latest after 24 hours.

1.4 Design

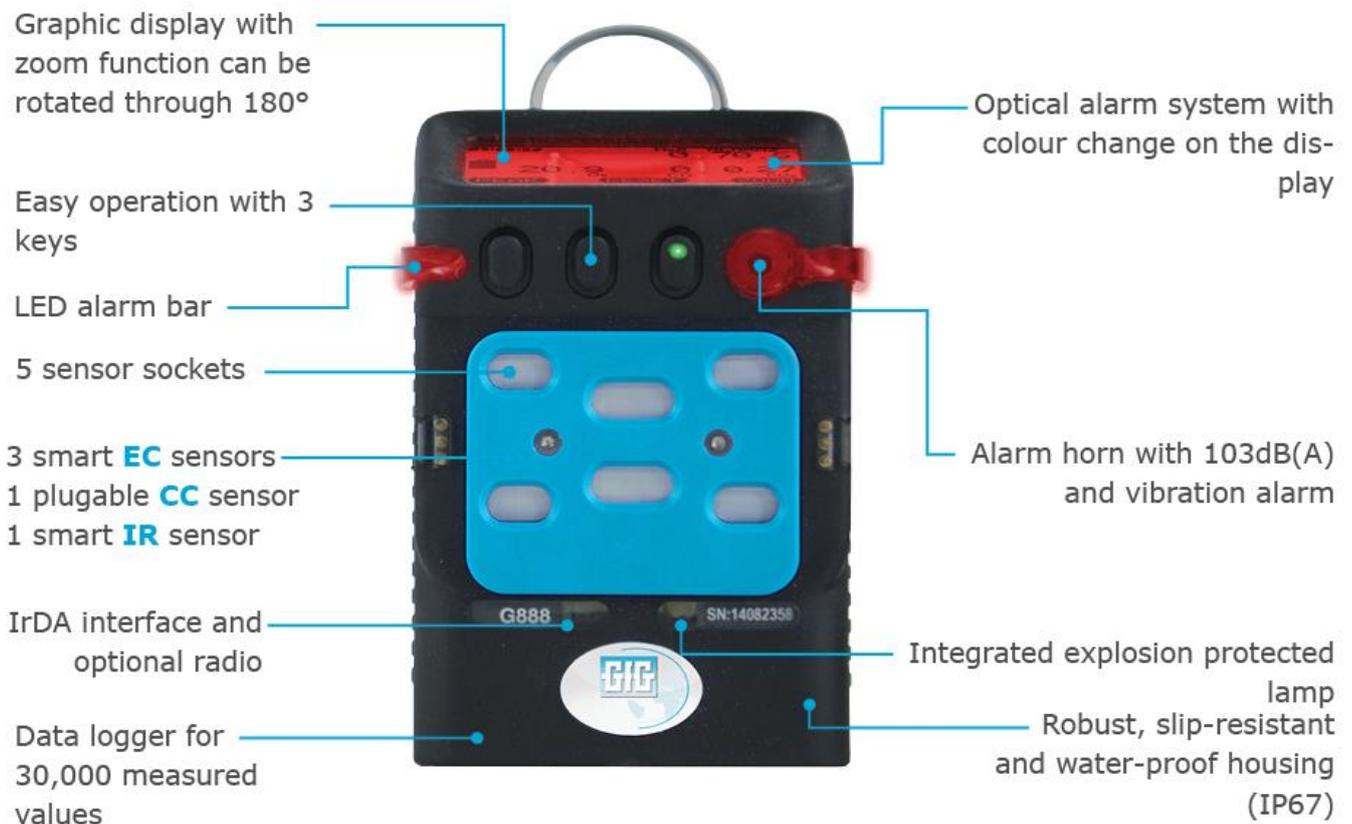

2 Operating Instructions

2.1 Commissioning

2.1.1 Switching the device on and off




Switch on the device by briefly pressing the right button .

Switch off the device by pressing the right button  for about 5 seconds. Release the button when the display "Switch off / 0" is shown.

When charging the device, the normal measuring mode is automatically switched off and the past charging time will be displayed.

After having switched off the device, it performs a **self-test** and gives information about the Firmware version, the built-in sensors with their measuring ranges and the alarm thresholds as well as the date of the next inspection. During the self-test, the visual and acoustical signal transmitters will be controlled in a way that the user would recognise a gas alarm.

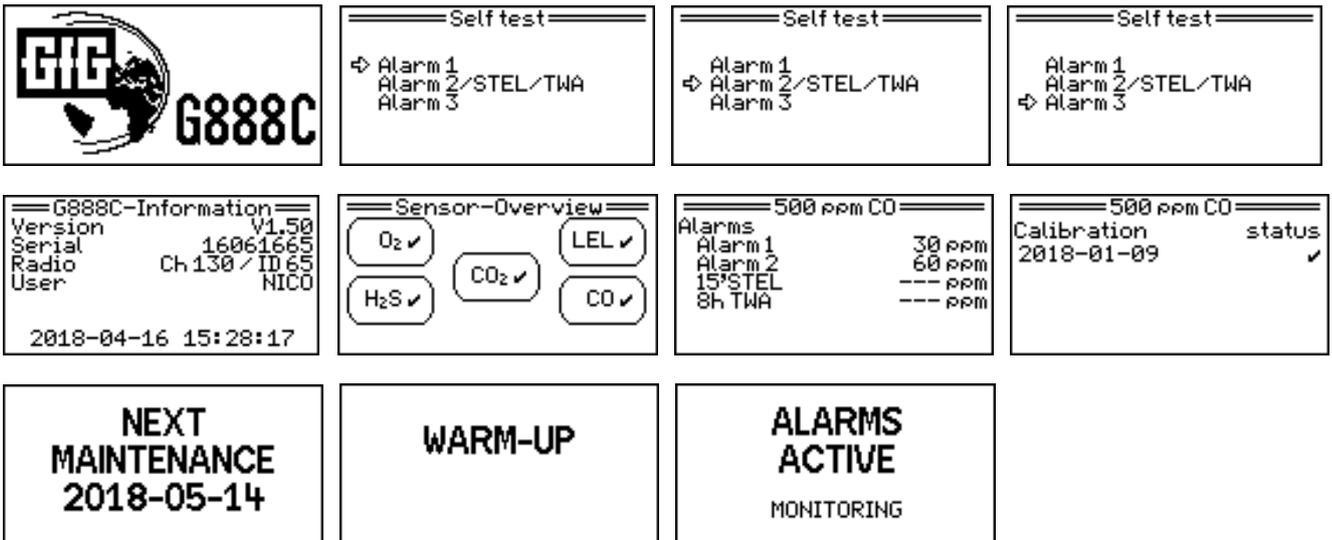


Alarm thresholds and calibration data will be displayed for all available sensors. Please find an example of CO below. Depending on the condition of the sensors, other messages will be output, which possibly need to be acknowledged. Please find more detailed information in the section "Other messages when starting the device".


After having switched on the device and the passing of the messages, the device will be ready for operation after about one minute. By pressing the centre button, it is possible to acknowledge displays and messages.

2.1.2 Other messages when starting the device


The G888 will test the sensors when starting the device and monitors the adjustment data. For a sensor, which had not been adjusted yet or which had been adjusted more than one year ago, the message "Sensor adjustment required!" will be the output. Since almost used up sensors might have a reduced adjustment interval in which case the message "Sensor adjustment or sensor replacement required!" will be the output. In case of used up sensors, the message "Sensor replacement required!" will be the output when the device would be started. These messages need to be acknowledged by pressing the button.

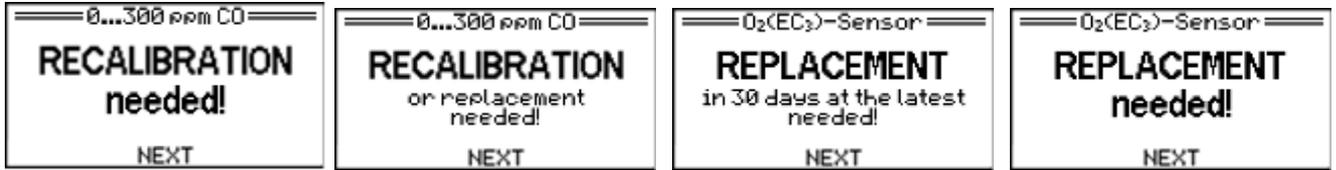

If a docking station is used to check the device, then the intervals for the functional test and for the sensor adjustment might have been set in the G888. The dates for the next functional test or the next sensor adjustment automatically result of the time of the last tests. Depending on what will be due next, the date of the next functional test or of the next sensor adjustment will be displayed when starting the device. If a date has already been exceeded, the G888 will notify this "overdueness". These messages need to be acknowledged by pressing the button.

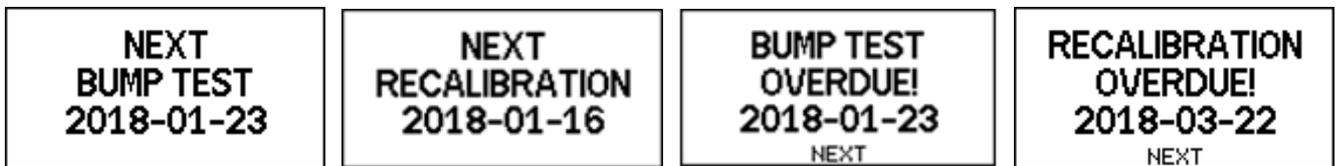


2.2 Measuring mode



The G888 is ready for operation if the time, the battery icon and all measured values are displayed with the measuring gas and the unit. It is monitored if the measured gas concentrations exceed the preset limit values and in case of oxygen it is monitored if the measured values fall below the preset limit values.

2.2.1 Display of the measured values, icons and key functions

Depending on the selected function or on the activated device option, also other icons can be displayed in the upper display row.





-  Motion detection (see section 2.2.5)
-  Flashlight (see section 2.2.10)
-  Peak display of peak values (see section 2.2.8)
-  Radio and field strength (see section 2.2.15)
-  Battery capacity (see section 2.2.4)

The current functions of the three keys are always displayed in the bottom display row. In this case, it is possible to switch the **PEAK** mode on and off by briefly pressing the left key. The gas alarms can be acknowledged by briefly pressing the centre key (**RESET**). It is possible to change over to the **ZOOM** display or to the detail view by briefly pressing the right key.

2.2.2 Monitoring and gas alarms

If the measured gas concentration exceeds (falls below 0) a preset limit value, an acoustical and visual alarm will be immediately emitted. It is possible to read from the display which gas has triggered the alarm. The alarm-triggering measured value is displayed inverted every second.



On the left in the picture, the alarm is triggered by a high CO₂ reading. In addition to the inverted display alternates "Vol CO₂" / "Alarm 2".

An extremely loud acoustical alarm (103dB(A) @30cm) and a bright visual all-round alarm provide for a safe warning in case of a gas hazard. In case of a gas alarm, the whole display will be coloured orange or red, depending on the alarm condition. The device has up to three alarm levels. The pre-alarm Alarm 1 is not self-holding, whereas the main alarms Alarm 2 and Alarm 3 are self-holding (factory setting). The G888 makes three limit value alarms available for oxygen and flammable gases (e.g. CH₄) and it makes two momentary value alarms available for toxic gases (e.g. CO, H₂S).

An exposition value alarm can additionally be emitted for the toxic gases if the long-term and the short-term exposure value (TWA and STEL) have been exceeded. Also refer to the sections "Alarm limit value - Basic setting" and "Alarms - Alarm setting". In addition, the alarming can be performed with a vibrator.


Type of alarm	Sensors	Number of alarms	Description
Momentary value (AL)	Oxygen	3	A momentary value alarm is immediately being triggered, if the gas concentration exceeds or falls below a preset value (O ₂). The momentary value alarms cannot be set.
	Flammable gases	3	
	Toxic gases	2	
short-term value (STEL)	Toxic gases	1	The short-term value (STEL) refers to a period of time of 15 minutes and the mean will be taken over this period of time. The STEL alarm is not self-holding. It will automatically switch off as soon as the short-term limit value falls below once again.
Long-term value (TWA)	Toxic gases	1	The long-term value (TWA) refers to a period of time of a working shift of 8 hours and the mean will be taken over this period of time. The TWA alarm cannot be reset. It will only be switched off, if the device is being switched off.

The alarms will be prioritised as follows: Power error, exceeding the measuring range, AL3, TWA > AL2, STEL > AL1, falling below the measuring range > temperature error.

2.2.3 Acknowledging the gas alarms

The momentary value alarms 2 and 3 are self-holding (factory setting) and can only be reset by pressing the button **RESET**, if it falls below or exceeds the preset limit values at O₂. The momentary value alarm 1 is not self-holding and will be automatically reset as soon as the alarm condition does no longer exist.

If the measuring range is exceeded on the catalytic combustion sensor (e.g. CH₄), for gas concentrations above 110 % LEL or above 5.5Vol.% CH₄ arrows **↑↑↑** showing upwards will be displayed instead of the gas display. The sensor will be deactivated in order that it will not be damaged. The alarm signalling and the arrows **↑↑↑** showing upwards will be maintained. The alarm signalling can only be terminated by pressing the button **RESET**. Then, the following questions will be displayed:



Only if it is made sure that **there is no flammable gas on the sensor, but only fresh air, the question may be answered with YES**. In this case, the sensor will be reactivated and will display measured values after a short running-in period!

Please find further details in the section "Peculiarities when monitoring the LEL range".

2.2.4 Battery capacity and battery alarm



In the measuring mode, the capacity of the battery can be read from the state of charge battery icon on the right of the display. The black filling represents the remaining capacity. By pressing the right button (**ZOOM**) several times, if required, it is also possible to display the remaining capacity as a figure. (*1)

Generally, the fully charged battery would have a capacity for a continuous operation of more than 7 hours (8...65 hours depending on the sensor combination - also refer to the technical data). The service life can be reduced by alarms. If the state of charge drops to such a low level that the state of charge icon is no longer filled out, the device will switch to the "Energy-saving mode". From this moment on, the green display lighting will no longer be activated when pressing a button. In case of a gas alarm, the red display lighting will also no longer be used. Then, the alarm signalling only occurs with the red alarm LEDs with a maximum horn volume of 90dB(A). If the state of charge drops even further, the battery alarm would be triggered and signalled acoustically. In this condition, the state of charge icon will flash. The maximum remaining service life is displayed in minutes. After 15 minutes, the device will automatically switch off with a clear acoustical signal. Then, the message "OFF" will be displayed for 5 minutes. If the function "Anti-Lazy-Battery" has been activated in the option menu, the device will not be automatically switched off after 15 minutes, but only when the minimum voltage falls below.

2.2.5 Motion detection and Man-Down Alarm

The G888 offers the option to monitor the movement of the device user. This option can be used for applications if no other person is within close proximity.



If the device user cannot act for himself any more, he can rapidly call for help by the acoustical alarm signalling or by radio.

If the motion detection is switched on, it is displayed in the top display row by the motion icon (☞).

If the internal motion sensor does not detect any motion during a defined period of time, an optical and acoustical MAN-DOWN-ALARM will be triggered after a warning time of 30 seconds. Then, this alarm can be reset by a keystroke. During the warning time, the timer can be reset by moving the device or by a keystroke.


If the device is equipped with a radio module, the motionless time and, if applicable, a triggered MAN-DOWN-ALARM will be transmitted together with the gas measurement values.

The motion detection is set in the service menu under System / System options / Man-Down-Alarm (see section 2.3.2.1.5).

2.2.6 Short-term, Long term, Maximum, Minimum values

After having switched on the device, it will continuously measure in the diffusion mode. All concentrations will be displayed in this operating mode. In addition, short-term and long term values (STEL and TWA) will be formed for toxic gases and maximum (MAX) and only for oxygen O₂ minimum (MIN) values will be saved. These saved values can be displayed on the screen if the screen is switched over to the corresponding display mode by pressing the right button **ZOOM**.

2.2.7 Zoom display and detail view



In order to be able to see the measured values magnified on the **Zoom** display, press the **right button (ZOOM)**. Briefly press the button in order to zoom a displayed value. By pressing the right button several times, you can zoom the display of the measured values of the individual sensors one after another.

When the display of a value is zoomed, you can long press the button **ZOOM** and change over to the following detail view:




Example: Detail view for CO₂

- Top left: Maximum value (since switching on or since the last RESET)
- Top right: Current gas concentration
- Bottom left: Short-term value (15 minutes)
- Bottom right: Long-term value (8 hours)

Within one session you can change between the two zoom modes by long pressing the button **ZOOM**. After having activated a zoom display, the display generally skips to the normal view after about 10 seconds, depending on the configuration (system options). If the button **RESET** is pressed in the zoom display, the maximum/minimum value memory will be reset to the current gas concentration.

2.2.8 Peak display of the peak values



It is possible to continuously display peak values in the peak mode which is activated by pressing the button **PEAK**. On the screen in the top row, the peak icon ∇ will be displayed with the two arrows.



The peak mode can be deactivated by pressing the button **PEAK**.



In the detail view of the zoom display on the top left the corresponding peak value is displayed instead of the max. or min gas concentration.

If the button **RESET** is pressed in the detail view, the peak value memory will be reset to the current gas concentration.


2.2.9 Turning the display



The G888 allows turning the measured value display by 180°. To do so, keep the left and right button pressed simultaneously and release it. In this way, the display can be easily read when the device is attached to the belt.

2.2.10 Use of the flashlight

It is reasonable to use the integrated flashlight e.g. if the device is lowered into a shaft or if it is used as a safe light source in dark potentially explosive areas.



The flashlight can be switched on by long pressing the left button (about 3 sec.) and it can be switched off by shortly pressing it.

The switched on flashlight is shown in the upper display line by the flashlight icon ∇ .

2.2.11 Display lighting

The display lighting is switched on by pressing any key for about 10 seconds and then it will automatically switch itself off. If the battery is quite heavily discharged, the display lighting will no longer be switched on when pressing a key.

2.2.12 Peculiarities when monitoring in the LEL range

For the monitoring of the LEL range, the G888 can be equipped with a sensor, which works according to the catalytic process (WT). Due to the measurement method, the G888 measured values in the LEL range cannot be distinguished from values in the increased Vol. % range (e.g. >20 Vol.% CH₄). Furthermore, the sensor would be damaged by concentrations above 110%LEL. In order to avoid such a damage, the sensor will be switched off if gas concentration above 110%LEL is being detected. Only by pressing the button **RESET** and confirming the question "Fresh air?" by pressing the button **YES** the sensor will be switched on again.

At an oxygen concentration of less than 10 Vol.% it would be no longer possible to measure flammable gases and vapours with the catalytic process (CC) without errors. Please find more details about this topic in the chapter "Influence of oxygen and interference gases".

2.2.13 Influence of oxygen and interference gases

For using the G888C with a pellistor, it is necessary to pay attention that the measurement for gas and / or vapour concentrations in the measurement range below 100% LEL cannot exactly be performed, if the oxygen concentrations are at the same time less than 10 Vol%. In this case, the oxygen which is necessary for the "catalytic combustion" is missing for the heat tone sensor. If the oxygen sensor would measure such a low concentration, question marks "???" will be displayed instead of the measured value in %LEL. If the oxygen concentration would increase above 10 Vol%, the measured value will be displayed correctly. The Ex approval does not apply for the use of the device in an oxygen-enriched atmosphere. Certain substances, which are designated as "Sensor or catalytic toxin" in the technical vocabulary, can impair the catalytic combustion sensor (CC) regarding its signal behaviour. The "sensitivity", i.e. the ability of the sensor to emit signals, decreases. Substances of this kind are for instance sulphur, lead and silicon compounds.

2.2.14 Recording of measurement data with the data logger


The measurement data can be recorded on the G888 with an internal data logger. No special activation of the data logging is required.

30.000 measuring points each can be recorded for up to 12 different measured values and other information. This includes date, time, measuring point, alarm triggering and special events.

In the menu item "data logger" of the service menu it is possible to set different functions of the data saving. It is possible to select the recording of average values, peak values or momentary value as well as the recording interval between 1 second and 60 minutes. The memory type is set to a ring memory at the factory. I.e. the oldest measured values will be overwritten as soon as the data logger is full. Measured data can be read with the help of a test station TS888/999 or a docking station DS400. The configuration of the data logger can be modified with the operating menu.

2.2.15 Wireless data transfer

If a corresponding radio module is built in the G888 and switched on, the current gas measurement values can also be requested and transferred by radio.

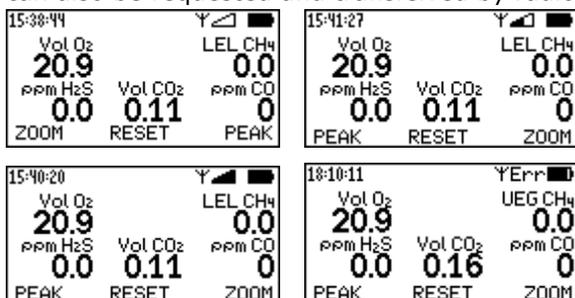

If the radio module is activated, the icons for radio and field strength are displayed in the upper display row. The stronger the field strength icon is filled in, the better is the radio connection. A flashing field strength icon signals that currently no measured values are requested or that the radio connection is interrupted. If the icon is displayed, the radio module is either defective or switched on but not existing at all.

Generally, the reach of the radio connection extremely depends on the structural circumstances between the sender and the receiver. At free visibility, a reach of 700m is possible with the 868MHz radio module. In buildings, the reach can considerably fall below 100m depending on the material, number and thickness of walls and other metallic components.

The device-specific setting of the radio address and also the radio channel is performed in the service menu under System / System options / Radio (refer to the paragraph 2.3.2.1.5).

2.3 Service mode

Access the service mode by pressing the centre button for about 3 seconds long **RESET**. In the service mode it is possible to set the G888 by modifying the program parameters. Some menu items can only be accessed via an access code "0011". The access code prevents that important functions might be accidentally modified or modified by unauthorised persons. An alarming cannot be performed in the service mode.

The main menu is the first menu item in the service mode.

2.3.1 Main menu


Menu control: The individual key functions will always be displayed by the labelling via the individual buttons on the screen.



Left button ↓ = Scrolling one menu item downward
Centre button **SELECT** = Choosing the highlighted menu item
Right button **DETECT** = Back to the measurement operation

The individual menu items in the main menu are:

2.3.1.1 Place – Choice of a measuring point



From a table stored in the device, it is possible to select one of 100 possible places. All table entries can only be edited with a PC. In a table entry it is possible to save up to 15 letters / figures, which are saved as "**Job site**" in the G888.




By pressing the left and centre button a stored place will be selected. The choice is automatically completed, when the selected value is confirmed with the right "Back" button.

2.3.1.2 Name – Choice of a device user



From a table stored in the device, it is possible to select one of 20 possible entries. All table entries can only be edited with a PC. In table entries it is possible to save up to 15 letters / figures, which are saved as "**Identification**" in the G888.



By pressing the left and centre button a stored user will be selected. The choice is automatically completed, when the selected value is confirmed with the right "Back" button.



2.3.1.3 AutoCal – Menu for AutoCal adjustment

In the menu item AutoCal several sensors can be simultaneously adjusted with fresh air (AIR) or test gas (GAS). Except from the CO₂ sensor, all sensors can be adjusted with fresh air without any further settings. When adjusting with test gas (GAS) the sensors need to be released depending on the used test gas / mixture. (Also refer to the paragraphs "AutoCal air . . ." and "AutoCal gas . . .")



The menu item AutoCal can be selected in the main menu or alternatively by simultaneously pushing the button in the middle and on the right one.



Then, the following functions can be chosen:
AIR = AutoCal adjustment with fresh air
GAS = AutoCal adjustment with test gas
EXIT = Back to the main menu



AutoCal adjustment with fresh air has been successful.




AutoCal adjustment with test gas mixture has not been successful. (e.g. due to wrong test gas concentration)

An AutoCal adjustment with fresh air is only performed if the sensor reading of the set point 0.0 (except for O₂) does not deviate more than ±10% from the measuring range or if the set point 20.9Vol.%O₂ does not deviate more than ±5.2Vol.%O₂. An AutoCal adjustment with test gas is only performed if the sensor reading of the "Cal.Gas" set point (in the sensor menu "Calibrate") does not deviate more than 25%. In case of larger deviations, the corresponding sensor will then be marked with "Error" in the subsequently indicated

AutoCal report. In this case, adjust the sensor in the sensor menu "Zero" or "Calibrate" or with the docking station.


The adjustment can be performed in the diffusion mode with fresh air exempt from measuring gas. However, no ambient air should be used for the zero point adjustment of the CO₂ sensor, since the ambient air always contains a small portion of carbon dioxide (CO₂) which would then result in wrong CO₂ measured values. For this reason, the zero point of the CO₂ sensor should only be adjusted in the sensor menu "Zero" or with the docking station with CO₂-exempted zero gas. It could be e.g. synthetic air, 100Vol%N₂ or specially purified air (CO₂-free). Zero gas (air exempted from measurement gas) and test gas can be supplied via the calibration cap "SMART CAP" with a volume flow from 0.5...0.6slpm (l/min).

2.3.1.4 Sensor overview

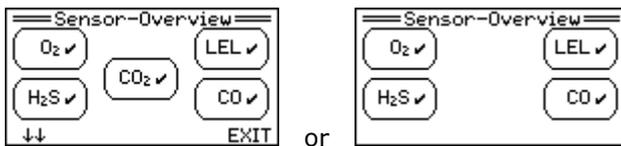


The sensors which are represented in the overview are located in the corresponding plug-in locations of the device.

Display of the alarm settings as well as date and status of the last calibration

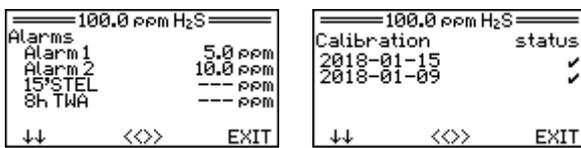

The data of the last three sensitivity adjustments can be displayed in the sensor menu "Calibration data". The status display indicates if they have been successful (✓) not faulty (✗).


Sensor information



In this menu item, specific information for each individual sensor are displayed:

- ID = Number of the measuring chamber
- SN = Serial number
- MR = Measuring range
- SE = Gas sensitivity of the sensor (100% = nominal)
- TR = Temperature range
- OT = Operating time of the sensor, e.g. 125 of 791 days

2.3.1.5 System information



In the system menu item **Information** you will find information about the device type, the firmware version, the serial number of the device.

2.3.2 Service menu

Access the service menu by selecting the main menu item **Service**. In the service menu it is possible to set the G888 by modifying the program parameters.

The menu items can only be accessed via an access code "0011". The access code prevents that important functions might be accidentally modified or modified by unauthorised persons. An alarming cannot be performed in the service mode.




- = Go to the next letter in the alphabet
- = Confirm letters (The cursor automatically skips to the next position). By long pressing the key, the last entry will be deleted, the cursor will skip one position back.




- = Go to the previous letter in the alphabet

After having entered the code 0011, the following will be displayed:



In the menu item **System** it is possible to perform general settings (refer to the section "System menu"). In the menu item **Sensors** it is possible to set sensor-specific functions (zero point and sensitivity adjustment). It is possible to retrieve information or to set alarm thresholds. By pressing the button **DETECT** you would exit the service menu and go back to the measuring mode.

2.3.2.1 System menu for system settings




These menu items are explained in the following paragraphs:


- Bumptest (see section 2.3.2.1.1)
- Sensor adjustment (zero point + calibration) (see section 2.3.2.1.2)
- Maintenance, setting the next date (see section 2.3.2.1.3)
- Time, setting date and time (see section 2.3.2.1.4)
- System options for diverse settings (see section 2.3.2.1.5)
- Sensor choice – Activation / deactivation (see section 2.3.2.1.6)
- AutoCal air, Sensor release for AutoCal adjust (see section 2.3.2.1.7)
- AutoCal gas, Sensor release for AutoCal adjust (see section 2.3.2.1.8)

2.3.2.1.1 Bump test


The functional test (inspection of the sensor values and alarms) can be easily and rapidly performed with the docking station DS400. The functional test is performed automatically, the intervals for the functional test will be stored in the G888. The functional test interval will be activated in the docking station after the first functional test.



Interval of the functional test is not activated.




Interval of the functional test is activated; the next functional test is immediately due.




Functional test on January 15th, 2018 was correct
Next functional test will be due 7 days later.

2.3.2.1.2 Sensor adjustment (zero point and calibration)

The sensor adjustment (zero point and calibration) can be easily and rapidly performed fully automatic with the docking station DS400. The intervals for the sensor adjustment will be saved in the G888 and activated from the docking station after the first sensor adjustment.



Sensor adjustment on March 19th, 2018 was correct. The interval of the functional test is not activated.



Sensor adjustment on March 19th, 2018 was correct.
The next sensor adjustment will be due 28 days later.

2.3.2.1.3 Maintenance

It is possible to enter a date in order not to forget the date for the next maintenance; the G888 will automatically trigger an alarm if this date is exceeded. After having exceeded the date, the G888 will inform the user that an maintenance needs to be performed as soon as the device is switched on.

To do so, it is necessary to select first **Maintenance** in the service menu.



It is possible to first select which parameter needs to be changed (year, month and day):

- EXIT** = Back to the system menu
- SELECT** = Selecting the parameter to be flashing
- >>** = Change over to the next parameter



The following options are available in order to modify a parameter:

- = Reduce value
- = Confirm value
- = Increase value

2.3.2.1.4 Time

The device has a clock for date and time. The clock is buffered by a lithium cell, which is designed for a useful life of 20 years.



In the **Time menu** the corresponding flashing parameter is selected with

- = Select.
- = Skip to the next parameter.
- = Go back to the system menu.




The following options are available in order to modify a parameter:

- = Reduce value
- = Confirm value
- = Increase value

2.3.2.1.5 System options

If "**System options**" is selected in the service menu, the following will be displayed:




- **Language** (Device language can be set e.g. German, English)
- **Contrast** (Display contrast can be set individually)
- **Volume** (Horn with 103dB(A), 90dB(A), 0dB(A))
- **Man-Down-Alarm** (see below)
- **Radio** (see below)
- **Tolerance band** (see below)
- **Vibrator** (on / off)
- **Start-up + AutoCal** (on / off)



Man-Down-Alarm



In the menu item "Man-Down-Alarm", it is possible to switch the motion detection on and off.



The "Motionless time" can be set from 20...300s. After the expiration of this time, the device user will be warned for 30 seconds. Only afterwards, the "Man-Down-Alarm" will be triggered in the measuring mode.

Radio-Adjustment

If a radio module is integrated in the G888, it is possible to switch the radio function on and off in the menu item "**Radio**". Depending on the radio module which is built in the G888, it will be displayed as (868MHz) or as (915MHz). If the radio module is switched on, it is possible to individually set the radio address and the radio channel. By default, the last two figures of the serial number of the device are being used. This corresponds to the setting (auto). Alternatively, the radio address can also be set from 0...254 (fixed). On the 868MHz radio module, the radio channel, which is by default set to 130, can also be set in the range from 101...111 or from 129...132. On the 915MHz radio module, no radio channel is being set, since this radio module is working with frequency hopping.




Switch tolerance band on/off

In the measuring mode, the G888 suppresses little fluctuations of the measuring value on sensors for toxic and flammable gases in the range of the zero point. In case of the oxygen measurement, low fluctuations about 20.9Vol% O₂ (fresh air range) will be suppressed. In order to avoid skips, the display value will be adjusted to the double value of the tolerance band up to the real measured value. Please find detailed information about the size of the tolerance band in the section "Sensor types and measuring ranges".

This tolerance band is activated by the manufacturer, but here under the system options it can generally be switched off as well. It is alternatively possible to enter the shortcut <REAL> for the deactivation or the shortcut <BAND> for the activation instead of the access code.

2.3.2.1.6 Sensor choice – activation / deactivation of sensors

Each sensor can be individually switched on or off for the measurement. This function will always be used if a gas shall not be measured or if a sensor is taken out of the device without replacing it.



On = Sensor active

Off = Sensor inactive


If no (gas) is indicated behind the sensor, the sensor is not available or it is not being identified.

↓ = Scroll downward to the next sensor

On/Off = Activate / deactivate the corresponding sensor

EXIT = Back to the service menu

2.3.2.1.7 AutoCal air - Sensor release for AutoCal adjustment



Here it is possible to set which sensors should be used for the automatic adjustment with fresh air.


Except for the IR sensor for CO₂ by default all sensors are set to "ON" and are this released for the automatic fresh air adjustment.

↓ = Scroll downward to the next sensor

On/Off = Adjustment / Non-adjustment of the sensor in the AutoCal program

EXIT = Back to the service menu

2.3.2.1.8 AutoCal gas sensor release for AutoCal adjustment



Here it is possible to set which sensors should be calibrated for the automatic adjustment with test gas. By default, all sensors are set to "OFF". If several sensors need to be adjusted simultaneously with a test gas mixture, these sensors can be selected here.

↓ = Scroll downward to the next sensor

On/Off = Adjustment / Non-adjustment of the sensor in the AutoCal program

EXIT = Back to the service menu

2.3.2.2 Sensor menu for sensor settings

The following functions refer to the individual sensors in the G888. In the sensor menu, each sensor can be selected individually. Then, the settings apply for each selected sensor.

For the description of the functions of the sensor-specific settings the CH₄ sensor resp. the O₂ sensor are mentioned as an example. However, the setting options apply for all sensors in the same way.



Input options:

↓ = Changing over to the next sensor

SELECT = Selecting the sensor

EXIT = Back to the service menu



The following settings are available for each sensor:

Zero = Adjusting the zero point

Calibrate = Adjusting the sensitivity

Alarms = Setting the alarm thresholds

Calibration data = Data and status of the last calibration and zeroing)

Information = Sensor information: MK number, serial number, measuring range, temperature range)


Unit and Type of gas = Selecting the CH₄ unit to be displayed (%LEL / Vol%) or selection of the type of gas to be displayed



- = Changing over to the next menu item
- = Selecting the menu item
- = Back to the service menu


2.3.2.2.1 Zero - Adjusting the zero point

When adjusting the zero point, the sensors should be gassed with air exempt from measuring gas or the carbon dioxide and the oxygen sensor (*1) with 100Vol% nitrogen. In this case, the zero gas can be supplied via the "SMART CAP" calibration cap with a flow from 0.5...0.6slpm (l/min). In order to adjust the zero point, it is necessary to select the sensor menu item "Zero". Then, the following will be displayed:




- = Starting the zero point adjustment
- = Inputting the zero gas concentration
- = Back to the "CH₄menu"

Generally, the zero gas is 0.0 so that it is not necessary to modify this concentration. However, in special cases, the zero gas concentration can be slightly raised after having pressed the button GAS. After having input **GAS** the following screen will be displayed:



- = Reducing the zero gas concentration by one unit
- = Confirming the value and back to the menu item "Zero"
- = Increasing the zero gas concentration by one unit

By inputting **Start** the zero point adjustment is being started:



- = Cancelling the adjustment and changing over to the "CH₄" menu.

If a constant measured value is registered after a stabilisation time of 100 seconds, the adjustment will be performed and conformed by pressing the button "OK". For CO, IR and O₂ sensors the stabilisation time is a bit longer but generally limited to 3 minutes.

For (*1): The zero point adjustment of the oxygen sensor will be performed with 100Vol% nitrogen at the factory. For the monitoring of the usual alarm thresholds of ≥17Vol.%O₂ no readjustment of the user would be needed. In this case, it is sufficient to adjust the sensitivity.


2.3.2.2.2 Calibrating - Sensitivity adjustment

The gas sensitivity of the sensor is adjusted for the calibration. Before performing the sensitivity adjustment, a zero point adjustment needs to be performed. A corresponding test gas is required for the sensitivity adjustment. Test gases are e.g.:

Measuring range	Test gas
TX	Carbon monoxide (CO), hydrogen sulphide (H ₂ S) or other gases
OX	Fresh air or test gas with 20.9 Vol% oxygen (O ₂) in nitrogen (N ₂)
EX	Methane (CH ₄), propane (C ₃ H ₈) or any other flammable gases (*2)

The test gases to be used can be learned from the test log. For the sensitivity adjustment, the concentration of the test gas should amount to from 30% to 70% of the measuring range end value. However, for IR sensors with measuring ranges of >5Vol.CO₂ the concentration of the test gas has to amount to from 25% to 75% of the measuring range end value. The test gas can be supplied via the "SMART CAP" calibration cap with a flow from 0.5...0.6slpm (l/min).

In order to adjust the sensitivity, it is necessary to select the sensor menu item "Calibrate".




- = Starting the sensitivity adjustment
- = Inputting the test gas concentration
- = Back to the "O₂" menu

By inputting the **GAS** the test gas concentration can be set in the range from 10 to 105% of the measuring range end value:



- = Reducing the test gas value by one unit
- = Increasing the test gas value by one unit
- = Confirming the value and back to the "O₂" menu

However, by inputting **Start** the sensitivity adjustment is being started:



- = Cancelling the adjustment a change over to the "O₂" menu.


If a constant measured value is registered after a stabilisation time of 25 seconds, the adjustment will be performed and conformed by pressing the button "OK". Generally, the stabilisation time is limited to 3 minutes.

For (*2): The sensitivity adjustment of sensors which measure certain flammable gases in the %LEL range, such as hexane, nonane or similar "heavy" vapours, is not unproblematic. Apart from the availability of such a test gas, it has to be assumed with a long stabilisation time in the range of several minutes for the gas supply. Alternatively, the sensitivity adjustment can be performed with a suitable reference gas (e.g. propane). The IR sensor MK249-8 can be adjusted e.g. with a reference gas of 0.85Vol%C₃H₈ (propane) to 67%LEL hexane or 80%LEL nonane. The cross-sensitiveness for such sensors are indicated in the section "Sensor specifications".

2.3.2.2.3 Alarms - Alarm setting

The G888 has 3 momentary value alarms for the non-toxic gases (O₂, CH₄) each, for the toxic gases (e.g. H₂S, CO, CO₂) there are 2 momentary value alarms each. The alarms are triggered if the gas concentration exceeds or falls below the corresponding limit value. An alarm can additionally be emitted for the toxic gases if the long-term and the short-term value (TWA and STEL) are being exceeded.

After having selected the sensor menu item **Alarms** the following screen is displayed (here: Selecting O₂):



- = Scroll downward
- = Selecting the menu item
- = Back to the sensor menu

After having selected the alarm limit value (in the example: Alarm 1) it is possible to enter the value:




The selected alarm limit value flashes and can only be changed, if:

- = Reducing the alarm value by one unit
- = Back to the sensor menu
- = Increasing the alarm value by one unit

With the exception of %LEL measuring ranges all limit values can be freely set or completely deactivated (0 or "---") over the whole measuring range. For %LEL measuring ranges, the limit values can be set to up to maximum 60%LEL.

2.3.2.2.4 Calibration data



In this menu item, the data of the last calibration will be displayed. It is a pure information display.

2.3.2.2.5 Information



The individual data of the sensors which are built-in the device, are displayed here.

- ID: The MK number corresponds to the sensor type
- SN: Serial number of the sensor
- MR: Measuring range of the sensor
- SE: Gas sensitivity of the sensor (nominal=100%)
- TR: Temperature range in which the sensor can be used

```

=====CH4(CC)-Info=====
ID: MK221-01
SN: 00000
NR: 100.0%LEL SE: 100%
TR: -25...65°C
OT: ???
PS: PowerSave Mode on
PS on/off EXIT

```

- OT: Operating time the sensor has already been used
 PS: The PowerSave mode from the Catalytic Sensor can be turned on or off with the left button. This mode cannot be activated if the sensitivity of the sensor is too low and on "heavier" gases (such as hexane, nonane or similar) due to the smaller sensor signal.

2.3.2.2.6 Measuring range

Under the menu item Measure range, different pre-defined measuring ranges are listed for smart GfG sensors. They can be selected.

```

=====Measuranger=====
100.0%LEL CH4
100.0%LEL H2
100.0%LEL C3H8
100.0%LEL C4H10
100.0%LEL C5H12
100.0%LEL nHexane
↓↓ SELECT EXIT

```

In this menu item (here WT sensor) it is possible to select the type of gas to be displayed or to set the CH₄ unit to %LEL or Vol.%. The volume concentration in brackets corresponds to the final value of the measuring range. Hereby it is possible to set the measuring range to the country-specific LEL value.

If the unit or the type of gas has been changed, the device needs to be restarted after quitting the service program, before performing a functional test or an AutoCal adjustment with a docking station.

2.3.2.3 Data logger settings

In the menu item **Data logger** it is possible to make different settings:

- Complete** - Deleting the data from the data logger (display of the memory usage)
- Mode** - Selection of momentary values, mean values or peak values
- Interval** - Interval of the data logging (selectable from 1 second to 60 minutes)

```

=====Data logger=====
Full 11%
Interval 00:01:00
Mode Average
Overwrite on
↓↓ ERASE EXIT

```

The parameter **COMPLETE** indicates how much capacity of the data logger has been completed.

- ↓** = Scrolling downward to the next parameter
- ERASE** = Deleting the data. A security query will follow "Delete data?". Confirm by pressing the button **YES** (right button), cancel by pressing the button **NO** (left button)

EXIT = Back to the main menu

```

=====Data logger=====
Full 11%
Interval 00:01:00
Mode Average
Overwrite on
↓↓ CHANGE EXIT

```

If the parameter **Mode** is selected by pressing the button **CHANGE**, it would be possible to choose between the momentary value, mean value and peak value (Peak). After having input **EXIT** the system will skip back to the logger menu. The selected mode will be taken over.

```

=====Data logger=====
Full 11%
Interval 00:01:00
Mode Average
Overwrite on
↓↓ CHANGE EXIT

```

Interval: The interval of the data logging can be selected by pressing the buttons on the left and right from 1 second to 60 minutes.

The data of the data logger can be read with the help of the charging tray or of the charging cap and an optional USB adapter cable and be transferred to a PC.

2.4 Energy supply

The G888 is equipped with a NiMH supply module as a device battery. In this supply module, the battery is an integral part of the back panel of the housing. A dangerous growth of dendrites, as it may happen e.g. in lithium polymer or lithium ion batteries, is excluded for the battery of the G888.

2.4.1 Charging the device battery



Caution:

The device must not be charged in potentially explosive atmospheres.
The charging contacts must not get dirty.
(Refer to the paragraph "Maintenance" in the annex)

The battery of the G888 can be charged in the **charging tray**. Perfect functioning is only guaranteed if the charging tray is lying or is fixed horizontally and the mounting bracket is correctly clammed in. Caution: Do not mount vertically!



Charging tray with mounting bracket

The charging tray will be supplied by a plug-in power supply made by the company GfG or alternatively via a vehicle charging cable made by the company GfG. The charging tray limits the charging voltage for the G888 to max. 6V.

The charging process is subdivided in normal and trickle charging. The continuously illuminated green LED indicates the operational readiness of the charging tray. The continuously illuminated yellow LED indicates the normal charging process and the flashing yellow LED indicates the trickle charging. If the yellow and the red LED are flashing alternately, the battery will first be discharged and then the charging process will be automatically started. If only the red LED is flashing, the charging tray is defective.

Make sure that the charging process will be indicated by the yellow LED and on the display after having inserted the G888 into the charging tray and closing the mounting bracket. Otherwise, there might possibly be contact problems. In case of a completely discharged battery, the charging process will take about 6 to 7 hours. Then, the charging tray will automatically switch over to the trickle charging so that an overloading of the battery will be excluded. Both states of charge will be displayed on the screen of the G888. After having switched over to the trickle charge, the battery will have at least 95% of its capacity. In order to attain a capacity of 100%, the battery module needs to be charged another 2 hours with trickle charging.

With the help of the charging tray and an optional USB adapter cable, the data of the G888 data logger can be read and transferred to a PC.

Alternatively, it is possible to charge the battery of the G888 with the help of the "SMART CAP". The SMART CAP needs to be fixed to the G888 with the clip connection on the side.



SMART CAP

The SMART CAP will be supplied by a plug-in power supply of the GfG. The SMART CAP limits the charging voltage for the G888 to max. 6V. It applies the same for the charging process and the signalling of the green and yellow LED, as described above for the use of the charging tray. At the start of loading, make sure that the loading process is indicated by the yellow LED and on the display (otherwise there might possibly be contact problems).

With the help of the SMART CAP and a USB cable, the data of the G888 data logger can be read and transferred to a PC.

In addition, the SMART CAP also allows calibrating the device. However, this cannot be performed during the charging process.

In order to permanently maintain the capacity of the NiMH battery, make sure that the battery can only be charged by using the charger depending on the useful life and frequency and the charger is not used as a storage place for weeks for the gas measurement device. Please find recommendations in the following table for the charging depending on the device usage.

	Device usage	Recommendation for the charging of the battery
1.	Daily for more than 3h	Charge after use
2.	Daily for less than 3h	Charge every 2nd or 3rd day
3.	Once per week	Charge 1 day before the next use
4.	Once per month for more than 3h	Charge after use as well as 1 day before the next use
5.	Once per month for less than 3h	Charge 1 day before the next use
6.	Once per calendar quarter or rarer	Charge after use as well as 1 day before the next use

For 4,5,6: If the device is rarely used, then the battery needs to be charged after use, since one part of the sensor electronics also needs to be supplied with energy even when the device is switched off. If the device has not been used for a very long period of time and the battery is completely discharged, then the device needs to be recharged about 1 day before the next use. A normally discharged battery will generally be charged to 95% of its normal capacity within about 6 hours charging mode. After another 2h trickle charging mode, the battery will be charged to 100% of its normal capacity. If in spite of the completely charged battery the normal device service life would not be attained, this might be caused due to the "lazy battery effect" (effect of the inertia of the battery). At this, the discharge behaviour changes in such a way that in spite of the completely charged battery the battery icon is empty relatively quickly and the device can nevertheless be operated for a long time.

2.4.2 Removal of the lazy battery effect on a device battery

On the NiMH supply units, the so-called "lazy battery effect" and thus a reduction of the service life of the device might occur after longer non-use, due to wrong charging behaviour, due to unfavourable device use or due to temperature conditions above 50°C. This may occur if the battery of the device has never been completely discharged or if the battery is charged too often or too long. It has to be avoided to start the charging process several times per day and that the device is permanently deposited in the charger for several days or weeks. The "lazy battery effect" can often be remedied by completely discharging the NiMH battery. However, in order that the battery would not be completely discharged, the device must not be manually switched off.

2.4.3 Replacing the device battery (NiMH supply unit)



Caution: The device must not be opened in potentially explosive areas and therefore the NiMH supply unit (battery) must not be changed. Since the battery is an integral part of the back panel of the housing, it is only allowed to replace it outside the potentially explosive area by a NiMH supply unit of the **same type**.

The device needs to be switched off, before replacing the NiMH supply unit. In order to remove the back panel of the housing, the four screws at the back need to be unscrewed and the whole NiMH supply unit needs to be pulled off to the rear.

3 Annex

3.1 Maintenance

Soiling of the device housing can be removed using a cloth dampened with water. Do not use solvents or cleaning agents! Particularly make sure that the outer charging contact surfaces of the G888 and the charging contact pins of the charging adapters are clean. In case of bad/incorrect contacting of the charging adapter, the NiMH battery will only be charged incompletely or not at all.

3.2 Maintenance and inspection

The maintenance and inspection includes a regular review and adjustment of the sensitivity and of the zero point. Moreover, the functioning of the device needs to be checked. Gas warning devices can behave in different ways depending on the environmental conditions. Thus, it is important to perform a test and an adjustment, if applicable, independent from the maintenance works (refer to the DIN EN 60079-29-2 paragraph 9.2 as well as the DGUV Information 213-057 (T 023) and DGUV Information 213-056 (T 021) of the BG RCI in Germany). This test includes the following inspections:

- Visual inspection regarding mechanical damages
- Visual inspection of the gas entry
- State of charge of the battery
- Display with zero gas and with test gas as well as alarm triggering

The response behaviour of oxygen sensors can be checked with a suitable test gas (<18Vol.% O₂) and with the help of the docking station, the "SMART CAP" calibration cap. In the simplest case, the response behaviour can also be checked with slowly exhaled air.

3.3 Maintenance - Repair

The DIN EN 60079-29-2 „... gas measurement devices – selection, installation, use and maintenance of devices for the measurement of flammable gases and oxygen“, the DIN EN 45544-4 „... Electrical devices for the direct detection and direct concentration measurement of toxic gases and vapours, Part 4: Guideline for the selection, installation, use and maintenance“ as well as the corresponding national sets of rules need to be considered.

In the sense of the "Explosion Protection Directive", the "BGR 500, Section 2.33" (formerly: Accident prevention regulations (UVV) gases), the maintenance includes the maintenance, inspection and repair of gas warning units. The applicable measures are described in the DGUV Information 213-057 (T 021) and 213-056 (T 023) the BG RCI. The functional test has to be performed before the first use and at least every 4 months and includes:

- Position of the zero point
- State of charge of the battery
- Diffusion paths
- Display with zero gas and standard test gas, if applicable, adjustment
- Alarm signal triggering, e.g. with alarm test gas
- Constantly amplified signal with standard test gas
- Response time

The test has to be performed by an expert and a written confirmation about the result has to be available. Generally, the restoration of the G888 has to be performed according to the instructions of the manufacturer by using original spare parts for the maintenance.

3.4 Calibration device

The device has to be supplied with test gas in order to control the sensitivity of the display. The diffusion openings can be covered with the help of the "SMART CAP" so that the test gas can be supplied to the sensors with a flow from 0.5...0.6slpm (l/min). Alternatively, for certain test gases, this inspection can also be performed with the docking station DS400.

Caution: Test gases, in particular toxic gases may pose hazards. Make sure that test gases are not inhaled. Working places, where devices are calibrated with test gas, need to be sufficiently ventilated depending on the type of gas, concentration and gas quantity. In particular cases, a gas extraction or a gas discharge is suitable. The safety notes on the test gas bottles as well as the safety data sheets of the test gases need to be observed in any case.

3.5 Inspection with the docking station DS400

The functional test required in the DGUV Information 213-057 (T 023) and 213-056 (T 021), as well as the adjustment of the G888 can be easily and rapidly performed with the docking station.

The functional test will be automatically started and performed fully automated. The effective time for a functional test amounts to about 20 seconds. The adjustment (sensor adjustment) will be started at an individual push of a button and completed within a few minutes. A green or red LED will indicate the test result. The detailed values are displayed on the device screen (functional test report, AutoCal air report, AutoCal gas report). No PC is required to perform the functional tests and the adjustment, all relevant data will be automatically saved on an SD card which is inserted in the docking station.

The first time, the functional test of the G888 needs to be performed, the interval for the functional test and the adjustment can be automatically activated on the docking station.

Before using the docking station, it is necessary to read and follow its operating instructions.



3.6 Malfunction, cause, remedy

	Malfunction / Message	Cause	Remedy
1.	Simultaneously flashing alarm LEDs and display off	Insufficient voltage supply Hardware or program execution error	Charge battery Call the GfG service
2.	Permanent "Boot loader" with red display lighting	Program memory defective	Transfer Firmware to the device Call GfG service, if necessary
3.	"ERROR! RAM"	Working memory defective	Switch device off and on
4.	"ERROR! EEP"	Device parameter memory defective	Call GfG service, if necessary
5.	"ERROR! BAT"	Battery voltage metering defective	
6.	"ERROR! ALG"	Program execution error / Algorithm	
7.	"Clock chip does not work!" "Time reset to ..."	Hardware defect	Acknowledge message Call GfG service, if necessary
8.	"Reset time to ..."	Clock not set or buffer battery is empty	Acknowledge message, set time Call GfG service, if necessary
9.	"Sensor defective!"	Sensor defective or not available	Switch device off and on Call GfG service, if necessary
10.	"Data incorrect!"	Sensor data are incorrect	Switch device off and on Call GfG service, if necessary
11.	"Reconnect sensor to EC1!"	EC sensor is connected to the wrong slot	Open device, reconnect sensor, then switch the device on again
12.	"Reconnect sensor to EC2 or EC3!"		
13.	"Sensor not available. Deactivate sensor in the system menu!"	Sensor not available.	Acknowledge message and switch off sensor in the service program Call GfG service, if necessary
14.	"CHECK ALARMS"	Sensor was replaced by another type	Check alarm setting in the service program and change it, if necessary
15.	"Gas type is not supported"	Gas type is not supported by the device or old Firmware version	Remove sensor perform Firmware update, if necessary
16.	"No sensors"	No sensors activated in the service program	Activate available sensors in the service program
17.	Gas display "START" ("STRT")	Sensor is still in the activation phase	Wait for some seconds
18.	Gas display "????"	Measuring with WT sensor is not possible, since oxygen display <10Vol%	If this occurs with fresh air, it is necessary to adjust or replace the oxygen sensor
19.	Gas display "----" / Error	No gas display, since the sensor is defective or the sensor data are incorrect	Deactivate the sensor in the service program Call GfG service, if necessary
20.	Gas display " "	Measured value underrange Clearly falling below the measuring range	Perform zero point adjustment

21.	Gas display " "	Measured value over range/excess available gas concentration is too high or high cross sensitivity (for EC sensor) or protective circuit activated (for WT sensor)	Leave the range of high gas concentration and acknowledge message for the WT sensor and confirm in the fresh air range
22.	Gas display "FAULT" ("FLT")	IR sensor signal is incorrect	If this happens repeatedly Call GfG service
23.	Gas display "TEMP" or "TEMP ERROR"	Sensor is operated outside the specified temperature range or hardware defect at 0°C<Ta<30°C	Go to a normal environmental temperature range Call GfG service, if necessary
24.	Gas display "POWER" or "POWER ERROR"	Energy supply of the sensor is disturbed	If this happens repeatedly Call GfG service
25.	Gas display "P+T"	See gas display "TEMP" and "POWER"	See above
26.	"Gas concentration is too high!"	When changing from the HI% range to the %LEL range the gas concentration is still above 5Vol%	Wait until the gas concentration has reduced to less than 5Vol% and repeat switchover.
27.	"No sensors released for AutoCal air (gas)"	No sensors released for the automatic fresh air or test gas adjustment	Release for the automatic adjustment in the service program Sensor(s)
28.	"Zeroing failed measured value too high" (too low)	Possibly measuring gas available or too positive (negative) zero point deviation	Perform zero point adjustment in the environment exempt from measuring gas Call GfG service, if necessary
29.	"Calibration failed Measured value too low" (too high)	Wrong test gas concentration or sensor sensitivity too low (too high)	Check test gas and set point Call GfG service, if necessary
30.	"Zeroing (calibration) failed Signal cannot be detected"	Extreme sensor signal deviation or hardware defect	Repeat process and call GfG service, if necessary
31.	"Saving failed"	Parameters cannot be saved when quitting the service program	Switch device off and on, then repeat the settings in the service program Call GfG service, if necessary

3.7 Accessories and spare parts

	Description	Order No
1.	G888/G999 SMART CAP (calibration cap)	1990210
2.	G888/G999 SMART CAP with USB cable (calibration cap and data transfer)	1990211
3.	G888/G999 SMART CAP with USB cable and EU plug-in power supply (5.0VDC/1.0A)	1990212
4.	DIC888/999-B Charging tray with brackets and EU plug-in power supply (12VDC/700mA)	1990221
5.	DIC888/999-B Charging tray with brackets and vehicle charging cable	1990222
6.	DIC888/999 USB interface cable	1990229
7.	DS400 Docking station for G888/G999-D with EU plug-in power supply (12VDC/1300mA)	1990231
8.	DS404 Docking station for G888/G999-D with EU plug-in power supply (12VDC/1300mA)	1990236
9.	TS888/999 Test station without fitting without plug-in power supply	1990240
10.	TS888/999 Test station with fitting without plug-in power supply	1990241
11.	TS888/999-DIC Test station with charging function without fitting without plug-in power supply	1990245
12.	TS888/999-DIC Test station with charging function with fitting without plug-in power supply	1990246
13.	G888C NiMH supply unit A21	1990401
14.	G888 Spare sensors → refer to the section "Sensor types and measuring ranges"	

The spare parts and the accessories need to be stored at an environmental temperature from 0° to 30°C. The storage time must not exceed 5 years. For NiMH supply units a shorter storage time of one year applies. The battery must be charged before the storage. If the device might be stored for more than ½ year, the battery should be removed.

3.8 Indications regarding the environmentally friendly disposal

According to section 11 of the General Terms and Conditions of the company GfG, the purchaser of the device agrees to dispose of the device or device components in an environmentally sound manner in line with sections 11 and 12 of the German Electrical and Electronic Equipment Act (ElektroG). If desired, GfG in Dortmund, Germany, can also carry out correct disposal.

3.9 Sensor types and measuring ranges

The spare sensors need to be stored at an environmental temperature from 0° to 30°C. The storage time must not exceed one year. For electrochemical sensors a shorter storage time of ½ year applies. When storing oxygen sensors, the service life to be expected will be reduced. When storing the spare sensors, make sure that the environmental atmosphere is not aggressive and free from sensor toxins.

Slot	Sensor type	Display range	Measuring gas and additional information	Order No
EC1	MK380-8	0 ... 500ppm 0 ... 100ppm	CO Carbon monoxide and H ₂ S hydrogen sulphide	1990710
EC1 EC2 EC3	MK390-8	0 ... 10ppm (*1)	Cl ₂ Chlorine	1990725
	MK391-8	0 ... 2ppm	ClO ₂ Chlorine dioxide	1990730
	MK349-8	0 ... 2ppm	COCl ₂ Phosgene	1990800
	MK443-8	0 ... 500ppm (*1)	CO Carbon monoxide	1990705
	MK445-8	0 ... 100ppm (*1)	H ₂ S Hydrogen sulphide	1990700
	MK396-8	0 ... 2000ppm	H ₂ Hydrogen	1990785
	MK402-8	0 ... 1Vol.%	H ₂ Hydrogen	1990790
	MK403-8	0 ... 4Vol.%	H ₂ Hydrogen	1990795
	MK409-8	0 ... 50ppm (*1)	HCN Hydrogen cyanide	1990760
	MK412-3	0 ... 10ppm	HF Hydrogen fluoride (EU version)	1990765
	MK412-9	0 ... 10ppm	HF Hydrogen fluoride (resolution 0.5ppm)	1990766
	MK453-8	0 ... 300ppm (*1)	NH ₃ Ammonia	1990735
	MK454-8	0 ... 1000ppm(*1)	NH ₃ Ammonia	1990740
	MK458-8	0 ... 30ppm (*1)	NO ₂ Nitrogen dioxide	1990750
	MK383-8	0 ... 25Vol.%	O ₂ Oxygen (2 years)	1990715
	MK427-8	0 ... 25Vol.%	O ₂ Oxygen (3 years)	1990716
	MK353-8	0 ... 10ppm (*1)	PH ₃ Phosphine	1990770
	MK460-8	0 ... 20ppm (*1)	SiH ₄ Silane	1990780
MK440-8	0 ... 10ppm (*1)	SO ₂ Sulphur dioxide	1990720	
EC2 EC3	MK379-8	0 ... 20ppm (*1)	C ₂ H ₄ O Ethylene oxide	1990775
	MK392-8	0 ... 30ppm (*1)	HCl Hydrogen chloride	1990755
	MK432-8	0 ... 25Vol.%	O ₂ Oxygen (5 years)	1990717
	MK457-8	0 ... 100ppm (*1)	NO Nitrogen monoxide	1990745
CC	MK221-0	0 ... 100%LEL	Flammable gases and vapours (*2)	1990850
		0 ... 5Vol.%	CH ₄ Methane	
IR (Infrared)	MK221-1	0 ... 100%LEL	Flammable gases (*2) (increased contamination resistance)	1990851
		0 ... 5Vol.%	CH ₄ Methane (increased contamination resistance)	
IR (Infrared)	MK245-1	0 ... 5Vol.%	CO ₂ Carbon dioxide	1990920
		0 ... 100%LEL	Flammable gases and vapours (*2)	
		0 ... 5Vol.%	CO ₂ Carbon dioxide	
IR (Infrared)	MK248-8	0 ... 5Vol.%	CO ₂ Carbon dioxide	1990900
		0 ... 100%LEL	Flammable gases and vapours (*2)	1990905

For (*1): The sensor can also be set to other measuring ranges (refer to the sensor specification)

For (*2): CH₄ Methane or one of the below mentioned flammable gases and vapours

Sensor type	Flammable gases and vapours
MK221-0	CH ₄ (methane), C ₃ H ₈ (propane), C ₄ H ₁₀ (butane), C ₅ H ₁₂ (pentane), C ₆ H ₁₄ (n hexane), H ₂ (hydrogen), C ₂ H ₂ (acetylene), C ₂ H ₄ (ethylene), CH ₄ O(methanole), C ₂ H ₆ O(ethanole), C ₃ H ₈ O(isopropanole), C ₄ H ₁₀ O(n butanole), C ₃ H ₆ O(acetone), C ₃ H ₆ O ₂ (methylacetate), C ₄ H ₈ O ₂ (ethylacetate), C ₄ H ₈ O(methylethylketone MEK), C ₇ H ₈ (toluene), C ₆ H ₁₂ O(methylisobutylketone MIBK), C ₇ H ₁₆ (heptane), C ₉ H ₂₀ (n nonane)
MK221-1	CH ₄ (methane), C ₃ H ₈ (propane), C ₄ H ₁₀ (butane), C ₅ H ₁₂ (pentane), C ₆ H ₁₄ (n hexane), H ₂ (hydrogen), C ₂ H ₂ (acetylene), C ₂ H ₄ (ethylene)
MK245-1 MK249-8	CH ₄ (methane), C ₃ H ₈ (propane), C ₆ H ₁₄ (n hexane), C ₉ H ₂₀ (n nonane), ETF (ethyl formate)

3.10 Sensor specification

MK221-0 Catalytic combustion sensor for flammable gases and vapours			
Measuring ranges:	0.0...100%LEL	0.00...5.00Vol.% CH4	
Resolution / tolerance band:	0.5 / ±2.5%LEL	0.02 / ±0.14Vol.% CH4	
Response time:	t ₅₀ ≤ 10sec	t ₉₀ ≤ 20sec	@ CH ₄ (methane)
	t ₅₀ ≤ 12sec	t ₉₀ ≤ 30sec	@ C ₃ H ₈ propane)
	t ₅₀ ≤ 25sec	t ₉₀ ≤ 65sec	@ C ₆ H ₁₄ (n hexane)
Pressure (70)80....120(130)kPa:	max. ±5(7)%LEL or ±10% of the display		(regarding 100kPa)
Humidity 0%...95% RH:	max. ±3%LEL or ±10% of the C ₃ H ₈ display		(regarding 0% RH @40°C)
	or ±30% of the CH ₄ display		(regarding 0% RH @40°C)
Temperature(-20)-10...+40(55)°C:	max. ±3%LEL or ±10(15)% of the display		(regarding 20°C)
Flow velocity 0...6m/s:	max. ±1%LEL or +15% of the display @Flow velocities ≥1,5m/s		
Cross sensitivities @ 50% LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u> <u>n-hexane display</u>
	2.00Vol.% H ₂	about 65%LEL	about100%LEL about 135%LEL(theor.)
	2.20Vol.% CH ₄	<u>= 50%LEL</u>	about 75%LEL about 100%LEL
	1.15Vol.% C ₂ H ₄	about 48%LEL	about 58%LEL about 77%LEL
	0.85Vol.% C ₃ H ₈	about 33%LEL	<u>= 50%LEL</u> about 65%LEL
	0.70Vol.% C ₄ H ₁₀	about 31%LEL	about 47%LEL about 62%LEL
	0.55Vol.% C ₅ H ₁₂	about 28%LEL	about 40%LEL about 52%LEL
	0.50Vol.% C ₆ H ₁₄	about 27%LEL	about 38%LEL <u>= 50%LEL</u>
	0.45Vol.% C ₇ H ₁₆	about 19%LEL	about 28%LEL about 35%LEL
	0.40Vol.% C ₈ H ₁₈	about 15%LEL	about 23%LEL about 29%LEL
	They can vary from one sensor to another and depend on the gas concentration as well as on the age of the sensor.		
Expected service life:	3 years in pure air		
MK221-1 Catalytic combustion sensor for flammable gases (with increased contamination resistance)			
Measuring ranges:	0.0...100%LEL	0.00...5.00Vol.% CH4	
Resolution / tolerance band:	0.5 / ±2.5%LEL	0.02 / ±0.14Vol.% CH4	
Response time:	t ₅₀ ≤ 10sec	t ₉₀ ≤ 20 sec	@ CH ₄ (methane)
	t ₅₀ ≤ 12sec	t ₉₀ ≤ 30 sec	@ C ₃ H ₈ (propane)
	t ₅₀ ≤ 40sec	t ₉₀ ≤ 105sec	@ C ₆ H ₁₄ (n-hexane)
Pressure (70)80....120(130)kPa:	max. ±5(7)%LEL or ±10% of the display		(regarding 100kPa)
Humidity 0%...95% RH:	max. ±3%LEL or ±10% of the C ₃ H ₈ display		(regarding 0% RH @40°C)
	or ±20% of the CH ₄ display		(regarding 0% RH @40°C)
Temperature(-20)-10...+40(55)°C:	max. ±3%LEL or ±10(15)% of the display		(regarding 20°C)
Flow velocity 0...6m/s:	max. ±1%LEL or +20% of the display @Flow velocities ≥1.5m/s		
Cross sensitivities @ 50% LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u> <u>n-hexane display</u>
	2.00Vol.% H ₂	about 65%LEL	about100%LEL about 135%LEL(theor.)
	2.20Vol.% CH ₄	<u>= 50%LEL</u>	about 75%LEL about 100%LEL
	1.15Vol.% C ₂ H ₄	about 48%LEL	about 58%LEL about 77%LEL
	0.85Vol.% C ₃ H ₈	about 33%LEL	<u>= 50%LEL</u> about 65%LEL
	0.70Vol.% C ₄ H ₁₀	about 30%LEL	about 47%LEL about 62%LEL
	0.55Vol.% C ₅ H ₁₂	about 26%LEL	about 40%LEL about 52%LEL
	0.50Vol.% C ₆ H ₁₄	about 25%LEL	about 38%LEL <u>= 50%LEL</u>
	They can vary from one sensor to another and depend on the gas concentration as well as on the age of the sensor.		
Expected service life:	3 years in pure air		
MK248-8/MK245-1 Infrared sensors for carbon dioxide CO₂			
Measuring range:	0.02...5.00Vol.%	or	0.00...25Vol.%
Resolution:	0.01...0.05Vol.%	or	0.01...0.5Vol.%
Response time:	t ₅₀ ≤ 20sec	t ₉₀ ≤ 50sec	t ₁₀ ≤ 50sec @ CO ₂
Pressure 70...130kPa:	<1.6% of the display per 1% pressure change		(regarding 100kPa)
Humidity 0%...95% RH:	max. ±0.01 Vol.% or ±2% of the display		(regarding 50%RH @20°C)
Temperature -20...+55°C:	max. ±0.02 Vol.% or ±10% of the display		(regarding 20°C)
Long term stability per month:	max. ±0.01 Vol.% or ±2% of the display		(under laboratory conditions)
Expected service life:	6 years		

MK249-8/MK245-1 Infrared sensors for flammable gases and vapours				
Measuring range:	0.0...100%LEL	0.00...100Vol.% CH ₄		
Resolution:	0.2...1.0%LEL	0.01...0.5Vol.% CH ₄		
Tolerance band:	±1.2%LEL	±0.05Vol.% CH ₄		
Response time:	t ₅₀ ≤ 20sec	t ₉₀ ≤ 45 sec @ CH ₄ (methane)		
	t ₅₀ ≤ 25sec	t ₉₀ ≤ 66 sec @ C ₃ H ₈ (propane)		
	t ₅₀ ≤ 30sec	t ₉₀ ≤ 99 sec @ C ₆ H ₁₄ (n hexane)		
	t ₅₀ ≤ 55sec	t ₉₀ ≤ 371sec @ C ₉ H ₂₀ (n nonane)		
Pressure	70...130kPa:	<1.5% of the CH ₄ display per 1% pressure change	(regarding 100kPa)	
		<1.2% of the C ₃ H ₈ display per 1% pressure change	(regarding 100kPa)	
Humidity	0%...95% RH:	max. ±2.0 %LEL or ±15% of the display	(regarding 0%RH @40°C)	
Temperature	-20...+50°C:	max. ±2.0 %LEL or ±10% of the C ₃ H ₈ display	(regarding 20°C)	
Cross sensitivities	@ 50%LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>
		0.85Vol% C ₃ H ₈	about 145%LEL	= 50%LEL
		1.20Vol% C ₂ H ₆	about 138%LEL	about 48%LEL
		0.70Vol% C ₄ H ₁₀	about 110%LEL	about 42%LEL
		1.00Vol% C ₃ H ₈ O	about 97%LEL	about 39%LEL
		0.50Vol% C ₆ H ₁₄	about 88%LEL	about 37%LEL
		0.55Vol% C ₅ H ₁₂	about 87%LEL	about 36%LEL
		0.45Vol% C ₇ H ₁₆	about 82%LEL	about 34%LEL
		1.00Vol% C ₄ H ₈ O ₂	about 69%LEL	about 31%LEL
		0.35Vol% C ₉ H ₂₀	about 65%LEL	about 31%LEL
		2.20Vol% CH ₄	= 50%LEL	about 26%LEL
		0.75Vol% C ₄ H ₈ O	about 41%LEL	about 22%LEL
		1.25Vol% C ₃ H ₆ O	about 26%LEL	about 16%LEL
		0.50Vol% C ₇ H ₈	about 26%LEL	about 16%LEL
		They can vary from one sensor to another and are depending on the gas concentration.		
Expected service life:	6 years			
MK349-8 Electrochemical sensor for phosgene COCl₂ (PGN)				
Measuring range:	0...2ppm			
Resolution / tolerance band:	0.01ppm / ±0.02ppm			
Response time:	t ₉₀ < 150sec			
Pressure	80...120kPa:	max. ±0.02ppm or ±10% of the display		(regarding 100kPa)
Humidity	10%...95% RH:	max. ±0.02ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+40°C:	max. ±0.02ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	ClO ₂ : -300%; HCl: 250%; AsH ₃ : 90%; Cl ₂ : 40%; NO ₂ : -10%; O ₃ : 10%; (*1)			
Expected service life:	1...1.5 years in air			
MK353-8 Electrochemical sensor for phosphine PH₃				
Measuring ranges:	0...10ppm	0...20ppm	0...50ppm	
Resolution / tolerance band:	0.05ppm / ±0.05ppm	0.05ppm / ±0.05ppm	0.05ppm / ±0.05ppm	
Response time:	t ₅₀ < 20sec	t ₉₀ < 60sec		
Pressure	80...120kPa:	max. ±0.05ppm or ±10% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±0.05ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature	-20...+50°C:	max. ±0.05ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	SiH ₄ :90%; GeH ₄ :90%; AsH ₃ :65%; B ₂ H ₆ :35%; SO ₂ :20%; CO:0,5%; H ₂ :0.1%; (*1)			
Expected service life:	2...3 years in air			
MK379-8 Electrochemical sensor for ethylene oxide C₂H₄O (ETO)				
Measuring ranges:	0...20ppm	0...50ppm	0...100ppm	
Resolution / tolerance band:	0.1ppm / ±0.3ppm	0.1ppm / ±0.3ppm	0.1ppm / ±0.3ppm	
Response time:	t ₅₀ < 30sec	t ₉₀ < 120sec		
Pressure	80...120kPa:	max. ±1ppm or ±15% of the display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±2ppm or ±15% of the display		(regarding 50%RH @20°C)
Temperature	(-20)0...+40[50]°C:	max. ±1[2]ppm or ±15(20)% of the display		(regarding 20°C)
Cross sensitivities:	CO≈40%; CH ₄ O≈150%; C ₂ H ₂ ≈125%; CH ₂ O≈120%; CH ₄ S≈100%; C ₂ H ₄ ≈80%; C ₂ H ₆ O≈55%; C ₄ H ₁₀ O≈40%; C ₇ H ₈ ≈20%; MEK≈10%; among others			
Expected service life:	2...3 years in air			
Running-in time:	4 minutes up to 7 days – depending on the interruption time			
MK380-8 Electrochemical sensor for carbon monoxide CO and hydrogen sulphide H₂S (COSH)				
Measuring ranges:	0...500ppm CO (at EC ₀)	0...100ppm H ₂ S (at EC ₁)		
Resolution / tolerance band:	1ppm / ±3ppm CO	0.2ppm / ±0.6ppm H ₂ S		
Response time:	t ₅₀ < 20sec	t ₉₀ < 50sec		
Pressure	80...120kPa:	max. ±3(1)ppm or ±7(10)% of the CO (H ₂ S) display		(regarding 100kPa)
Humidity	15%...90% RH:	max. ±3(1)ppm or ±7(10)% of the CO (H ₂ S) display		(regarding 50%RH @20°C)
Temperature	-20...+50°C:	max. ±3(1)ppm or ±15(10)% of the CO (H ₂ S) display		(regarding 20°C)
Cross sensitivities	CO display:	H ₂ S:0...40%; H ₂ ≈20%; SO ₂ <20%; NO ₂ <2%; NO<0.3%; Cl ₂ :0%; (*1)		
Cross sensitivities	H ₂ S display:	CO<2%; NO ₂ ≈20%; SO ₂ :8...20%; NO<3%; H ₂ :0.03%; Cl ₂ :0%; (*1)		
Expected service life:	3 years in air			

MK383-8 Electrochemical sensor for oxygen O₂			
Measuring range:	0...25Vol.%		
Resolution / tolerance band:	0.1Vol.% / ±0.3Vol.%		
Response time:	t ₂₀ ≤ 6sec t ₉₀ ≤ 20sec		
Pressure 80...120kPa:	max. ±0.2 Vol% or ±2.5% of the measuring range		(regarding 100kPa)
Humidity 0%...90% RH:	max. ±0.2 Vol% or ±2.5% of the measuring range		(regarding 50%RH @40°C)
Temperature -20...+50°C:	max. ±0.5 Vol% or ±2.5% of the display		(regarding 20°C)
Expected service life:	2 years in air		
MK390-8 Electrochemical sensor for chorine Cl₂			
Measuring ranges:	0...10ppm	0...20ppm	0...40ppm
Resolution / tolerance band:	0.05ppm / ±0.10ppm	0.05ppm / ±0.10ppm	0.1ppm / ±0.1ppm
Response time:	t ₅₀ < 10sec t ₉₀ < 30sec		
Pressure 80...120kPa:	max. ±0.2ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	ClO ₂ :50%; F ₂ :40%; NO ₂ :20%; O ₃ :20%; SO ₂ :18%; CO ₂ :0%; CO:0%; H ₂ S:0%; H ₂ :0% (*1)		
Expected service life:	2...3 years in air		
MK391-8 Electrochemical sensor for chlorine dioxide ClO₂ (CLO)			
Measuring range:	0...2ppm		
Resolution / tolerance band:	0.01ppm / ±0.03ppm		
Response time:	t ₉₀ < 120sec		
Pressure 80...120kPa:	max. ±0.05ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±0.05ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.05ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	Cl ₂ ≈60%; O ₃ :-280%; H ₂ S:-25%; H ₂ : 0%; CO: 0%; (*1)		
Expected service life:	1...2 years in air		
MK392-8 Electrochemical sensor for hydrogen chlorine HCl			
Measuring ranges:	0...30ppm	0...50ppm	
Resolution / tolerance band:	0.2ppm / ±0.4ppm	0.2ppm / ±0.4ppm	
Response time:	t ₅₀ < 30sec t ₉₀ < 90sec		
Pressure 80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity 10%...95% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±1ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	AsH ₃ :350%; PH ₃ :300%; H ₂ S:65%; NO:45%; SO ₂ :40%; HCN:35%; Cl ₂ :6%; NO ₂ :3%; NH ₃ :0.1%; CO:0%; CO ₂ :0%; H ₂ :0%; (*1)		
Expected service life:	2...3 years in air		
MK396-8 Electrochemical sensor for hydrogen H₂ (*2)			
Measuring range:	0...2000ppm		
Resolution / tolerance band:	2ppm / ±50ppm		
Response time:	t ₅₀ < 30sec t ₉₀ < 90sec		
Pressure 80...120kPa:	max. ±10ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±10ppm or ±10% of the display		(regarding 50%RH)
Temperature -20...+50°C:	max. ±20ppm or ±20% of the display		(regarding 20°C)
Cross sensitivities:	C ₂ H ₄ ≈80%; NO≈35%; HCN≈30%; CO<20%; H ₂ S<20%; NO ₂ =SO ₂ =Cl ₂ =HCl=0%; (*1)		
Expected service life:	2...3 years in air		
MK402-8 Electrochemical sensor for hydrogen H₂ (*2)			
Measuring range:	0...1.00 Vol%		
Resolution / tolerance band:	0.01 Vol% / ±0.02 Vol%		
Response time:	t ₅₀ < 40sec t ₉₀ < 70sec		
Pressure 80...120kPa:	max. ±0.01 Vol % or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±0.01 Vol% or ±10% of the display		(regarding 50%RH)
Temperature -20...+50°C:	max. ±0.02 Vol% or ±20% of the display		(regarding 20°C)
Cross sensitivities:	NO ₂ :-400%; CO:150%; H ₂ S:20%; C ₂ H ₄ :yes; NH ₃ =CO ₂ =Cl ₂ =SO ₂ =HCN=0%; (*1)		
Expected service life:	2...3 years in air		
MK403-8 Electrochemical sensor for hydrogen H₂ (*2)			
Measuring range:	0...4.00 Vol%		
Resolution / tolerance band:	0.01 Vol% / ±0,05 Vol%		
Response time:	t ₅₀ < 40sec t ₉₀ < 60sec		
Pressure 80...120kPa:	max. ±0.01 Vol% or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±0.01 Vol% or ±10% of the display		(regarding 50%RH)
Temperature -20...+50°C:	max. ±0.02 Vol% or ±25% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S:220%; C ₂ H ₄ :yes; NH ₃ =CO ₂ =CO=Cl ₂ =HCN=NO=NO ₂ =0%; (*1)		
Expected service life:	2...3 years in air		

MK409-8 Electrochemical sensor for hydrogen cyanide HCN				
Measuring ranges:	0...50ppm	0...100ppm		
Resolution / tolerance band:	0.1ppm / ±0.5ppm	0.2ppm / ±1.0ppm		
Response time:	t ₅₀ < 25sec	t ₉₀ < 60sec		
Pressure 80...120kPa:	max. ±0.5ppm or ±10% of the display		(regarding 100kPa)	
Humidity 10%...95% RH:	max. ±0.5ppm or ±10% of the display		(regarding 50% RH @20°C)	
Temperature -20...+50°C:	max. ±0.5ppm or ±15% of the display		(regarding 20°C)	
Cross sensitivities:	NO ₂ ≈70%, NO≈-5%, H ₂ S≈0...200% (depending on the filter saturation)			
	CO=CO ₂ =H ₂ =0% (*1)			
Expected service life:	2 years in air			
MK412-3/MK412-9 Electrochemical sensors for hydrogen fluoride HF				
Measuring ranges:	0...10ppm	0...10ppm		
Resolution / tolerance band:	0.1ppm / ±0.3ppm (MK412-3)	0.5ppm / ±0.5ppm (MK412-9)		
Response time:	t ₅₀ < 40sec	t ₉₀ < 90sec		
Pressure 80...120kPa:	max. ±0.2ppm or ±10% of the display		(regarding 100kPa)	
Humidity 10%...80% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)	
Temperature -20...+40°C:	max. ±0.2ppm or ±10% of the display		(regarding 20°C)	
Cross sensitivities:	HCl:66%; Cl ₂ :40%; CO=CO ₂ =NO ₂ =H ₂ S=H ₂ =0% (*1)			
Expected service life:	1..2 years in air			
MK427-8 Electrochemical sensor for oxygen O₂				
Measuring range:	0...25 Vol%			
Resolution / tolerance band:	0.1 Vol% / ±0.3 Vol%			
Response time:	t ₂₀ ≤ 8sec	t ₉₀ ≤ 25sec		
Pressure (70)80...120(130)kPa:	max. ±0.4(0.6)Vol.% or ±2(3)% of the measuring range		(regarding 100kPa)	
Humidity 0%...95% RH:	max. ±0.5Vol.% or ±2.5% of the measuring range		(regarding 50%RH @40°C)	
Temperature (-20)-10...+55°C:	max. ±0.5(0.8)Vol.% or ±2.5(4.0)% of the display		(regarding 20°C)	
Expected service life:	3 years in air			
MK432-8 Electrochemical sensor for oxygen O₂				
Measuring range:	0...25 Vol%			
Resolution / tolerance band:	0.1 Vol% / ±0.3 Vol%			
Response time:	t ₂₀ ≤ 8sec	t ₉₀ ≤ 25sec		
Pressure 70...130kPa:	max. ±0.3 Vol% or ±3.0% of the display		(regarding 100kPa)	
Humidity 15%...90% RH:	max. ±0.5 Vol% or ±3.0% of the display		(regarding 50%RH @40°C)	
Temperature -20...+50°C:	max. ±0.5 Vol% or ±3.0% of the display		(regarding 20°C)	
Expected service life:	5 years in air			
MK440-8 Electrochemical sensor for sulphur dioxide SO₂				
Measuring ranges:	0...10ppm	0...20ppm	0...50ppm	0...100ppm
Resolution:	0.05ppm	0.05ppm	0.1ppm	0.1ppm
Tolerance band:	±0.15ppm	±0.20ppm	±0.3ppm	±0.4ppm
Response time:	t ₅₀ < 10sec	t ₉₀ < 30sec		
Pressure 80...120kPa:	max. ±0.2ppm or ±5% of the display		(regarding 100kPa)	
Humidity 15%...90% RH:	max. ±0.3ppm or ±3% of the display		(regarding 50%RH @20°C)	
Temperature -20...+50°C:	max. ±0.3ppm or ±5% of the display		(regarding 20°C)	
Cross sensitivities:	C ₂ H ₂ <300%; NO ₂ <-170%; C ₂ H ₄ <90%; HCN<50%; Cl ₂ <-40%; NO<10%; H ₂ S<0,4%; CO<0,4%; H ₂ <0,3%; NH ₃ =0%; (*1)			
Expected service life:	3 years in air			
MK443-8 Electrochemical sensor for carbon monoxide CO				
Measuring ranges:	3...500ppm	3...1000ppm	3...2000ppm	
Resolution / tolerance band:	1ppm / ±3ppm	1ppm / ±3ppm	1ppm / ±3ppm	
Response time:	t ₅₀ < 10sec	t ₉₀ ≤ 30sec	t ₁₀ < 30sec (decay time)	
Pressure 80...120kPa:	max. ±3ppm or ±10% of the display		(regarding 100kPa)	
Humidity 15%...95% RH:	max. ±3ppm or ±5% of the display		(regarding 50%RH @20°C)	
Temperature -20...+40(55)°C:	max. ±3ppm or ±5(10)% of the display		(regarding 20°C)	
Cross sensitivities:	C ₂ H ₄ ≈96%, C ₂ H ₂ ≈90%, H ₂ <30%(typ.15%), NO<20%, Cl ₂ <7%, C ₂ H ₆ O<0.5%, SO ₂ =NH ₃ =H ₂ S=0% (*1)			
Expected service life:	3 years in air			
MK445-8 Electrochemical sensor for hydrogen sulphide H₂S				
Measuring ranges:	0.2...50ppm	0.2...100ppm	0.2...200ppm	0.5...500ppm
Resolution:	0.1ppm	0.1ppm	0.2ppm	0.5ppm
Tolerance band:	±0.5ppm	±0.5ppm	±1.0ppm	±1.5ppm
Response time:	t ₅₀ < 10sec	t ₉₀ < 30sec	t ₁₀ < 30sec (decay time)	
Pressure 80...120kPa:	max. ±0.2ppm or ±5% of the display		(regarding 100kPa)	
Humidity 15%...90% RH:	max. ±0.2ppm or ±5% of the display		(regarding 50%RH @20°C)	
Temperature -20...+40(55)°C:	max. ±0.2ppm or ±5(10)% of the display		(regarding 20°C)	
Cross sensitivities:	NO ₂ <10%, CO<2%, NO<1%, CO ₂ =SO ₂ =Cl ₂ =NH ₃ =C ₂ H ₄ =0% little Methanol cross sensitivity (*1)			
Expected service life:	3 years in air			

MK453-8 Electrochemical sensor for ammonia NH₃			
Measuring ranges:	0...300ppm	0...500ppm	
Resolution / tolerance band:	1ppm / ±3ppm	1ppm / ±3ppm	
Response time:	t ₉₀ < 45sec		
Pressure 80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±1(2)ppm or ±15(20)% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈120%, NO ₂ ≈-100%, SO ₂ ≈-30%, CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)		
Expected service life:	2..3 years in pure air		
MK454-8 Electrochemical sensor for ammonia NH₃			
Measuring ranges:	0...500ppm	0...1000ppm	0...1500ppm
Resolution / tolerance band:	2ppm / ±5ppm	5ppm / ±10ppm	5ppm / ±10ppm
Response time:	t ₉₀ < 60sec		
Pressure 80...120kPa:	max. ±5ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±5ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+55°C:	max. ±10ppm or ±20% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈140%, NO ₂ ≈-100%, SO ₂ ≈-30%, CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)		
Expected service life:	2..3 years in pure air		
MK457-8 Electrochemical sensor for nitrogen monoxide NO			
Measuring ranges:	0...50ppm	0...100ppm	0...200ppm
Resolution / tolerance band:	0.2ppm / ±1.5ppm	0.5ppm / ±2.0ppm	0.5ppm / ±2.0ppm
Response time:	t ₅₀ < 15sec	t ₉₀ < 45sec	(at 20°C)
Pressure 80...120kPa:	max. ±1ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±1ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+40(50)°C:	max. ±2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S<50%; NO ₂ <40%; C ₂ H ₆ O±10%; SO ₂ <5%; H ₂ <1%; NH ₃ <1%; CO<-1%; CO ₂ =CL ₂ =0; (*1)		
Expected service life:	3 years in air		
Running-in time:	3 minutes to 1 day – depending on the interruption time		
MK458-8 Electrochemical sensor for nitrogen dioxide NO₂			
Measuring ranges:	0...30ppm	0...50ppm	0...100ppm
Resolution / tolerance band:	0.1ppm / ±0.3ppm	0.1ppm / ±0.5ppm	0.1ppm / ±0.5ppm
Response time:	t ₅₀ < 10sec	t ₉₀ < 30sec	(at 20°C)
Pressure 80...120kPa:	max. ±0.2ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.2ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	Cl ₂ ≈100%; H ₂ S<-40%; NO<20%; C ₂ H ₆ O<1%; CO<-1%; SO ₂ <-1%; H ₂ <-1%; NH ₃ <-1%, CO ₂ =0; (*1)		
Expected service life:	3 years in air		
MK460-8 Electrochemical sensor for silane SiH₄			
Measuring ranges:	0...20ppm	0...50ppm	
Resolution / tolerance band:	0.1ppm / ±0.2ppm	0.1ppm / ±0.2ppm	
Response time:	t ₅₀ < 20sec	t ₉₀ < 60sec	
Pressure 80...120kPa:	max. ±0.1ppm or ±10% of the display		(regarding 100kPa)
Humidity 15%...90% RH:	max. ±0.2ppm or ±10% of the display		(regarding 50%RH @20°C)
Temperature -20...+50°C:	max. ±0.3ppm or ±10% of the display		(regarding 20°C)
Cross sensitivities:	H ₂ S≈160%, PH ₃ ≈100%; SO ₂ ≈20%; H ₂ =CO=0%; (*1)		
Expected service life:	2..3 years in air		

For (*1): Gas display regarding the supplied concentration in the range of AGW (MAK) values

For (*2): Not permitted for the monitoring of the lower explosion limit for applications of the primary explosion protection

3.11 Alarm limit values - Basic setting

Basic setting of the alarm thresholds for toxic gases without exposure alert

Measuring range	Alarm 1	Alarm 2	STEL (15')	TWA (8h)
0 ... 20ppm C ₂ H ₄ O (ETO)	2.0ppm	4.0ppm	-	-
0 ... 10ppm Cl ₂	0.5ppm	1.0ppm	-	-
0 ... 2ppm ClO ₂ (CLO)	0.2ppm (*1)	0.4ppm		
0 ... 2ppm COCl ₂ (PGN)	0.1ppm	0.2ppm		
0 ... 500ppm CO	30ppm	60ppm	-	-
0 ... 5,0Vol.% CO ₂	0.5Vol.%	1.0Vol.%	-	-
0 ... 100ppm H ₂ S	5.0ppm	10ppm	-	-
0 ... 30ppm HCl	5.0ppm (*1)	10ppm	-	-
0 ... 50ppm HCN	5.0ppm (*1)	10ppm	-	-
0 ... 10ppm HF	1.0ppm	2.0ppm	-	-
0 ... 300ppm NH ₃	20ppm	40ppm	-	-
0 ... 100ppm NO	2.5ppm (*1)	5.0ppm	-	-
0 ... 30ppm NO ₂	2.0ppm (*1)	4.0ppm	-	-
0 ... 10ppm PH ₃	0.3ppm (*1)	0.6ppm	-	-
0 ... 20ppm SiH ₄ (SIL)	5.0ppm	10ppm	-	-
0 ... 10ppm SO ₂	1.0ppm	2.0ppm	-	-

For (*1): A monitoring of the AGW value is not satisfactory possible with the available sensor technology.

Basic setting of the alarm thresholds for toxic gases with exposure alert

Measuring range	Alarm 1	Alarm 2	STEL (15')	TWA (8h)
0 ... 20ppm C ₂ H ₄ O	2ppm	6ppm	4ppm	2ppm
0 ... 10ppm Cl ₂	1.0ppm	1.5ppm	1.0ppm	0.5ppm
0 ... 2ppm ClO ₂	0.2ppm	0.4ppm	0.2ppm	0.1ppm
0 ... 2ppm COCl ₂	0.1ppm	0.2ppm	0.2ppm	0.1ppm
0 ... 500ppm CO	30ppm	120ppm	60ppm	30ppm
0 ... 5.0Vol.% CO ₂	0.5Vol.%	2.0Vol.%	1.0Vol.%	0.5Vol.%
0 ... 100ppm H ₂ S	5.0ppm	15ppm	10ppm	5.0ppm
0 ... 30ppm HCl	5.0ppm	10ppm	5.0ppm	2.0ppm
0 ... 50ppm HCN	5.0ppm	10ppm	5.0ppm	1.9ppm
0 ... 10ppm HF	1.0ppm	3.0ppm	2.0ppm	1.0ppm
0 ... 300ppm NH ₃	20ppm	80ppm	40ppm	20ppm
0 ... 100ppm NO	2.5ppm	5.0ppm	2.5ppm	0.5ppm
0 ... 30ppm NO ₂	2.0ppm	4.0ppm	2.0ppm	0.5ppm
0 ... 10ppm PH ₃	0.3ppm (*1)	0.4ppm	0.2ppm	0.1ppm
0 ... 20ppm SiH ₄	5.0ppm	15ppm	10ppm	5.0ppm
0 ... 10ppm SO ₂	1.0ppm	3.0ppm	2.0ppm	1.0ppm

For (*1): A monitoring of the AGW value is not satisfactory possible with the available sensor technology.

Basic setting of the alarm thresholds for oxygen and for flammable gases and vapours

Measuring range	Alarm 1	Alarm 2	Alarm 3
0 ... 25Vol.% O ₂	19.0Vol.% (↓)	17.0Vol.% (↓)	23.0Vol.% (↑)
0 ... 2000ppm H ₂ (*2)	1000ppm	1500ppm	2000ppm
0 ... 1.0/4.0Vol.% H ₂ (*2)	0.40Vol.%	0.60Vol.%	0.80Vol.%
0 ... 5.0Vol.% CH ₄	1.00Vol.%	2.00Vol.%	3.00Vol.%
0 ... 100%LEL CH ₄ (*3)	20.0%LEL	40.0%LEL	60.0%LEL

For (*2): Not permitted for the monitoring of the lower explosion limit for applications of the primary explosion protection.

For (*3): or another of the following listed flammable gases and vapours

LEL values according to the DIN EN 60079-20-1:2010			
4.0Vol.% H ₂	hydrogen	(CAS-No.1333-74-0)	6.0Vol.% CH ₄ O methanol (CAS-No.67-56-1)
4.4Vol.% CH ₄	methane	(CAS-No.74-82-8)	3.1Vol.% C ₂ H ₆ O ethanol (CAS-No.64-17-5)
2.3Vol.% C ₂ H ₂	acetylene	(CAS-No.74-86-2)	2.5Vol.% C ₃ H ₆ O acetone (CAS-No.67-64-1)
2.3Vol.% C ₂ H ₄	ethylene	(CAS-No.74-85-1)	3.1Vol.% C ₃ H ₆ O ₂ methyl acetate (CAS-No.79-20-9)
2.4Vol.% C ₂ H ₆	ethane	(CAS-No.74-84-0)	2.7Vol.% C ₃ H ₆ O ₂ ethyl formate ETF (CAS-No.109-94-4)
1.7Vol.% C ₃ H ₈	propane	(CAS-No.74-98-6)	2.0Vol.% C ₃ H ₈ O isopropyl (CAS-No.67-63-0)
1.4Vol.% C ₄ H ₁₀	butane	(CAS-No.106-97-8)	1.5Vol.% C ₄ H ₈ O methyl ethyl ketone MEK (CAS-No.78-93-3)
1.1Vol.% C ₅ H ₁₂	pentane	(CAS-No.109-66-0)	2.0Vol.% C ₄ H ₈ O ₂ ethyl acetate (CAS-No.141-78-6)
1.0Vol.% C ₆ H ₁₄	n-hexane	(CAS-No.110-54-3)	1.4Vol.% C ₄ H ₁₀ O n-butanol (CAS-No.71-36-3)
0.85Vol.% C ₇ H ₁₆	heptane	(CAS-No.142-82-5)	1.2Vol.% C ₆ H ₁₂ O Methyl isobutyl ketone MIBK (CAS-No.108-10-1)
0-70Vol.% C ₉ H ₂₀	n-nonane	(CAS-No.111-84-2)	1.0Vol.% C ₇ H ₈ toluene (CAS-No.108-88-3)

3.12 Technical data

Type designations:	G888C	
Measuring principle:	Electrochemical (EC):	For toxic gases and oxygen
	Catalytic combustion (CC):	For flammable gases and vapours (up to 100%LEL)
	Infrared (IR):	For flammable gases and vapours and carbon dioxide
Measuring ranges:	refer to the section "Sensor types and measuring ranges" and "Sensor specification"	
Response time:	refer to the section "Sensor specification"	
Sensor service life:	refer to the section "Sensor specification"	
Measuring gas supply:	above the diffusion opening	
Display:	illuminated LCD full graphics display, automatic size setting for optimum reading, display of the battery capacity, gas concentration as current value and peak value	
Alerting:	depending on the gas type 3 or 2 momentary value and 2 exposure level alarms, battery alarm with visual and acoustical signalling as well as display on the screen, colour of the display depending on the alarm state (orange/red) Horn: 103 dB(A) (can be reduced to 90 dB(A))	
Zero point and sensitivity adjustment:	manual or automatic with an adjustment program, if necessary, test gas supply via the "SMART CAP" with 0.5...0.6slpm	
Radio:	optionally 868MHz for EU;	Range about 700m (free field)
	optionally 915MHz for US;	Range about 300m (free field)
Energy supply:	NiMH battery module; 2.6V 2100mAh; rechargeable	
Operating time (*1)		
	Without radio:	about 13h (EC+CC _{PS} +IR) about 9h (EC+CC+IR)
		about 21h (EC+CC _{PS}) about 13h (EC+CC)
		about 65h (EC) about 23h (EC+IR)
	With radio:	about 10h (EC+CC _{PS} +IR) about 7.5h (EC+CC+IR)
		about 14h (EC+CC _{PS}) about 10h (EC+CC)
		about 26h (EC) about 15h (EC+IR)
Climatic conditions		
	For operation:	-20...+50°C 5...95%RH 70...130kPa
	For storage:	-25...+55°C 5...95%RH 70...130kPa (recommended 0...+30°C)
Housing	Material:	rubberised polycarbonate
	Dimensions:	68 x 100 x 39mm (W x H x D)
	Weight:	up to 275g (depending on the sensor equipment)
	Protection class:	IP67
Approvals / Tests		
	Markings and Ignition protection type:	G888C Ⓢ I M2 Ex ia db I Mb Ⓢ II 2G Ex ia db IIC T4 Gb -20°C≤Ta≤+50°C
	EU Type examination certificate:	BVS 15 ATEX E 064 X
	IECEX Certificate of Conformity:	IECEX BVS 15.0056 X
	Electromagnetic Compatibility:	EN 50270:2015 Emitted interference: Type class I Interference resistance: Type class II

For (*1): The service life is indicated for new battery modules at operating temperatures of +20°C. It will be reduced by pressing buttons (display lighting & lamp) and by gas alarms. It is reduced with the age of the battery module, with the number of the charging / discharging cycles, by longer storage of the gas measurement device in the charging tray and the lazy battery effect.
CC_{PS}= Catalytic sensor with activated PowerSave mode if a reading of 0% LEL is detected. This energy saving mode can only be activated for certain measuring ranges (see section 2.3.2.2.5).

GfG Gesellschaft für Gerätebau mbH Klönnestraße 99; D-44143 Dortmund Phone: +49 (0)231 – 564 00-0 Fax: +49 (0)231 – 51 63 13 Internet: www.gfg.biz E-Mail: info@gfg-mbh.com			
Firmware Version 1.50	215-000.30_OM_G888.doc	Dated: June 29th, 2018	Subject to change without notice.

EU Declaration of Conformity GfG Gesellschaft für Gerätebau mbH

G888C, G888S

Klönnestraße 99
44143 Dortmund
Tel: +49 (231) 56400-0
Fax: +49 (231) 516313
E-Mail: info@gfg-mbh.com
www.gfg.biz



Edited: 31.07.2017 Amended: 02.03.2018

GfG Gesellschaft für Gerätebau mbH develops produces and sells gas sensors and gas warning devices which are subject to a **quality management system** as per DIN EN ISO 9001.

Subject to supervision by means of a **quality system**, surveilled by the notified body, DEKRA EXAM GmbH (0158), is the production of electrical apparatus of instrumentation Group I and II, categories M1, M2, 1G and 2G for gas sensors, gas detectors, gas warning systems in types of protection flameproof enclosures, increased safety, encapsulation and intrinsic safety, as well as their measuring function.

The portable detector **G888C, G888S** complies with directive **2014/34/EU** (ATEX) for devices and protective systems for proper use in potentially explosive atmospheres, directive **2014/30/EU** for electromagnetic compatibility, directive **2014/53/EU** (RED) relating to the making available on the market of radio equipment and with directive **2011/65/EU** (RoHS) on the restriction of the use of certain hazardous substances in electrical and electronic equipment.

For electrical explosion protection BVS 15 ATEX E 064 X
Labelling G888C: Ⓜ II 2G Ex ia db IIC T4 Gb / Ⓜ I M2 Ex ia db I Mb
Labelling G888S: Ⓜ II 2G Ex ia db IIC T4 Gb / Ⓜ I M1 Ex ia I Ma

The directive 2014/34/EU is complied considering the following standards:

- Explosive atmospheres
- General requirements EN 60079-0 : 2012 +A11 :2013
- Flameproof enclosure "d" EN 60079-1 : 2014
- Intrinsic safety "i" EN 60079-11 : 2012
- Group1, category-M1-equipment EN 50303 : 2000

The rating of the danger of ignition was done and documented. The EC-Type Examination Certificate was issued by the notified body with ID number 0158 (DEKRA EXAM, Dinnendahlstraße 9, D-44809 Bochum).

The directive 2014/30/EU is complied considering the following standard:

- Electromagnetic compatibility - Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen EN 50270 : 2015
- Emitted interference Type class 1
- Interference immunity Type class 2

The EMC test laboratory AMETEK CTS Germany GmbH at Kamen has tested and certified the electromagnetic compatibility.

The directive 2014/53/EU is complied considering the following standards:

- Short Range Devices (SRD) operating in the frequency range 25 MHz bis 1000 MHz EN 300220-2 V3.11 : 2017

Reference to the directive 2014/30/EU:

- ElectroMagnetic Compatibility (EMC) standard for radio equipment and services
- Common technical requirements EN 301489-1 V2.2.0 : 2017

Reference to the directive 2014/35/EU:

- Assessment of the compliance of low power and electronic and electrical equipment with the basic restrictions related to human exposure to electromagnetic fields (10 MHz – 300GHz) EN 62479 : 2010
- Information technology equipment- safety General requirements EN 60950-1: 2006 + A11: 2009 + A1: 2010 + A12: 2011 + AC: 2011 + A2: 2013

The test laboratory m.dudde hochfrequenz-technik, Bergisch Gladbach has tested and certified the compatibility.

The directive 2011/65/EU is complied considering the following standard:

- Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances EN 50581 : 2012

Dortmund, 06 March 2018

B. Siebrecht
B. Siebrecht
QMB

ATEX EU-RoHS-01604046

Translation

EU-Type Examination Certificate Supplement 3

- 1
- 2 **Equipment intended for use in potentially explosive atmospheres Directive 2014/34/EU**
- 3 EU-Type Examination Certificate Number: **BVS 15 ATEX E 064 X**
- 4 **Product:** Gas detector Type G888C Type G888S Type G999C Type G999S Type G999E Type G999P
- 5 **Manufacturer:** GfG Gesellschaft für Gerätebau mbH
- 6 **Address:** Klönnestr. 99, 44143 Dortmund, Germany
- 7 This supplementary certificate extends EU-Type Examination Certificate No. BVS 15 ATEX E 064 X to apply to products designed and constructed in accordance with the specification set out in the appendix of the said certificate but having any acceptable variations specified in the appendix to this certificate and the documents referred to therein.
- 8 DEKRA EXAM GmbH, Notified Body number 0158, in accordance with Article 17 of Directive 2014/34/EU of the European Parliament and of the Council, dated 26 February 2014, certifies that this product has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of products intended for use in potentially explosive atmospheres given in Annex II to the Directive. The examination and test results are recorded in the confidential Report No. BVS PP 15.2110 EU.
- 9 Compliance with the Essential Health and Safety Requirements has been assured by compliance with:
EN 60079-0:2012 + A11:2013 General requirements
EN 60079-1:2014 Flameproof enclosure "d"
EN 60079-11:2012 Intrinsic Safety "i"
- 10 If the sign "X" is placed after the certificate number, it indicates that the product is subject to the Special Conditions for Use specified in the appendix to this certificate.
- 11 This EU-Type Examination Certificate relates only to the design and construction of the specified product. Further requirements of the Directive apply to the manufacturing process and supply of this product. These are not covered by this certificate.
- 12 The marking of the product shall include the following:

II 2G Ex ia db IIC T4 Gb for type G888C, G999C, G999S
I M2 Ex ia db I Mb
Ⓜ II 2G Ex ia db IIC T4 Gb for type G888S
I M1 Ex ia I Ma
II 1G Ex ia IIC T4 Ga for type G999E, G999P
I M1 Ex ia I Ma

DEKRA EXAM GmbH
Bochum, 2018-01-02

Signed: Jörg Koch

Signed: Dr. Franz Eickhoff

Certifier

Approver



Page 1 of 3 of BVS 15 ATEX E 064 X / N3
This certificate may only be reproduced in its entirety and without any change.

DEKRA EXAM GmbH, Dinnendahlstraße 9, 44809 Bochum, Germany,
telephone +49 234 3696-105, fax +49 234 3696-110, tx-exam@dekra.com

13 Appendix

14 EU-Type Examination Certificate

BVS 15 ATEX E 064 X
Supplement 3

15 Product description

15.1 Subject and type

The Gas detector is modified according to the descriptive documents as mentioned in the pertinent test and assessment report and receives then the marking:

Gas detector type G888C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb
Gas detector type G888S	Marking:	II 2G Ex ia db IIC T4 Gb	I M1 Ex ia I Ma
Gas detector type G999C	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb
Gas detector type G999S	Marking:	II 2G Ex ia db IIC T4 Gb	I M2 Ex ia db I Mb
Gas detector type G999E	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma
Gas detector type G999P	Marking:	II 1G Ex ia IIC T4 Ga	I M1 Ex ia I Ma

15.2 Description

Reason for the supplement:

The Gas detector type G888 was renamed to type G888C. (No technical changes)
 The Gas detector type G889 was renamed to type G888S. (No technical changes)
 The Gas detector type G998 was renamed to type G999C. (The electronic circuit was slightly modified.)
 The Gas detector type G999 was renamed to type G999S. (The electronic circuit was slightly modified.)
 The Gas detectors type G999E and type G999P were added.
 The standard EN 50303:2000 is no longer applied. The EPL Ma requirements for the Gas detector are compiled by the standards listed on page 1.

Description of Product:

The Gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P is a portable instrument with a built-in power-supply battery. It is used for the detection of gases in ambient air under atmospheric conditions.

The Gas detector type G888C, type G888S, type G999C or type G999S contains 3 electro-chemical cells, 1 IR-sensor and 1 sensor of Flameproof Enclosure.

The Gas detector type G999E contains 4 electro-chemical cells and 1 IR-sensor.

The Gas detector type G999P contains 3 electro-chemical cells, 1 IR-sensor and 1 PID-sensor.

The measurement values are shown on a built-in display. If the present limits are reached, a visual alarm, an audible alarm and a vibrating alarm are produced.

A radio module for wireless data transfer can be optionally used inside of the Gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P.

The gas detector type G888C, type G888S, type G999C, type G999S, type G999E or type G999P is powered by a NiMH battery which has to be charged only outside of the hazardous area.

The gas detector type G999C, type G999S, type G999E or type G999P contains additionally a built-in pump.

Listing of all components used referring to older standards (optionally used in type G888C, G999C, G999S)

Subject and type	Certificate	Standards
Gas Sensor type A	Sira 07ATEX1088X	EN 60079-0:2006 EN 60079-1:2004

15.3 Parameters

15.3.1 Power supply battery in type G888C or type G888S

Nominal voltage	2.6 V
Nominal capacity	2100 mAh
Maximum charging voltage	U _m DC 6 V

15.3.2 Power supply battery in type G999C or type G999S or type G999E or type G999P

Nominal voltage	3.2 V
Nominal capacity	2100 mAh
Maximum charging voltage	U _m DC 9 V

15.3.3 Optionally radio module

Frequency range (depend on module type)	865.0 – 868.6 MHz or 865.0 – 870.0 MHz or 902.0 – 92.0 MHz
Nominal RF output power	< 35 mW
Maximum RF output power	< 250 mW
Ambient temperature range	-20 °C ≤ T _a ≤ +50 °C

16 Report Number

BVS PP 15.2110 EU, as of 2018-01-02

17 Special Conditions for Use

The measuring function according to annex II paragraph 1.6.5 of the directive 2014/34/EU is not part of this supplement to the EU-type Examination Certificate.

For Gas detector type G888C, G999C, G999S / usage Group I / mining:

The gas detector may only be used in potentially explosive atmospheres as intended. That means, that the device has to be carried on the body or has not to be discarded unattended, so that mechanical stress by impact is avoided. It is intended for the low risk of mechanical danger according to EN 60079-0.

The gas detector has to be immediately removed from the hazardous area and has to be cleaned when it is contaminated with oils and greases or hydraulic fluids.

18 Essential Health and Safety Requirements

The Essential Health and Safety Requirements are covered by the standards listed under item 9.

19 Drawings and Documents

Drawings and documents are listed in the confidential report.

We confirm the correctness of the translation from the German original.
In the case of arbitration only the German wording shall be valid and binding.

DEKRA EXAM GmbH
Bochum, dated 2018-01-02
BVS-Rip/Nu A 20170400

Certifier

Approver